Section	Page No.
Microinjection	
Introduction to Microinjection	298
Pico Injection/Micromanipulation System, PLS-1	299
Pico-Injector Systems, PLI-100	300 - 301
Pico-Injector Systems, PLI-90	302
PLI-100 & PLI-90 Injector Accessories	303
Multi-Channel Pressure Injection System, PM-8 & PM-4	304 - 305
ZonaDrill™ Laser System	306
Nanoject II/Auto Nanoliter Injector	307
SLAM Micropipettes	308
Chemical Drilling Micropipettes	309
Screw-Actuated Micrometer Driven Hamilton Syringe	310
Screw-Actuated Air Syringe	310
Tissue Sampling	
Vibratome® Tissue Sectioning System	311 - 313
Automatic Oscillating Tissue Slicer, EMS 4000	314 - 315
McIlwain Mechical Tissue Chopper	316
Microscopes	
Stereo Zoom Microscopes, SZM 180	317
Inverted Microscope, 900 Series	318
Illuminators	
Intralux 5100 Fiber Optic Cold Halogen Light Sources	319
V-Lux 1000 Fiber Optic Cold Light Source	320
Intralux IWL-500e Fiber Optic Cold Light Source	320
Intralux DC 1100 Fiber Optic Cold Light Source	321
Light Source Filters	321
Spare Lamps and Power Cords	322
Ring Light Adapters	322
Fiber Optic Ringlights	323 - 326
Gooseneck Light Guides	327 - 328
Articulating Arm and Modular Accessory System	329
Glass Light Fiber Backlights	330
Brightfield/Darkfield Base	330

PLI-100,
see page 300

Vibratome® 1000 Classic,
see page 311

SZM 180,
see page 317

Intralux 5100,
see page 319

Introduction to Microinjection

The use of Glass Needle (Fine Glass Microcapillary Pipette) based techniques for intracellular/extracellular microinjection and perfusion has become a popular procedure in numerous areas of experimental biology research (e.g. In vitro fertilization, transgenics, etc.). These techniques can best be described as micro surgical procedures that are conducted on a single cell using either a single or multiple barrel glass micropipette a precision positioning device (micromanipulator) and a microinjector or microperfusor. The micropipettes used in these procedures are formed using a Pipette Puller. The capillary glass tubing is heated to its softening point and 'pulled' to create the proper size tip diameter and taper for the desired application. The small tip diameters (as low as 0.2 µm) of these micropipettes combined with the high precision of the Micromanipulator and Microinjection/Perfusion Apparatus, allows for precise and accurate delivery. This precision allows for accurate and repeatable injections down to the sub-picoliter liter range into or around various types and sizes of cells with accuracy to 0.1 micron. The process of extruding substances through these micropipettes is accomplished through the use of either direct hydrostatic pressure (Pressure Injection) or by moving charged ions that are the result of an applied electric field (Iontophoresis) without the use of hydraulic flow.

Applications of microinjection range from assisted (In vitro) cell fertilization techniques to the transport of molecular and cellular elements. These substances are typically injected into the cell to manipulate and/or monitor the fundamental biochemistry of a specific living cell. Substance that can be injected include, cellular organelles, kinases, histochemical markers (such as horseradish peroxidase or lucifer yellow), proteins, metabolites, microbeads, ions, antibodies, genes, molecular biology mRNA and DNA, etc. The precise delivery (microperfusion) of small volumes (picoliter to milliliter) of various agents and drugs to a cell or group of cells for applications such as pharmacological drug testing can also be accomplished using these techniques.

In order for the researcher to conduct any of the above experiments and get meaningful results, the tools (equipment) used in these experiments must provide not only the specific functionality, but they also need to be of the highest quality and provide the necessary reliability, accuracy and repeatability to insure proper results. Harvard Apparatus, Inc. manufactures and sells the complete range of product that are needed to successfully microinject and/or microperfuse.

Warner and Harvard Apparatus Clark Capillary Glass, pages 214 to 220

Harvard Apparatus/Medical Systems Picoliter Injectors, pages 299 to 303

Harvard/Apparatus Medical Systems NeuroPhore, visit www.harvardapparatus.com for more information.

Pressure Injection Systems, pages 304 and 305

Pipette Pullers, pages 221 and 226

Micromanipulators, pages 244 to 256

PLS-1

Pico Injection/Micromanipulator System

The **PLS-1** Pico Injection/Micromanipulator System combines our popular PLI-100 pico injector, a motorized micromanipulator, and magnetic base in a single package.

The PLI-100 Pico-Injector delivers a wide range of volumes through micropipettes by applying a regulated pressure for a set period of time. The system features 5 pressures: inject, balance, clear, fill, and hold. The injector comes complete with input and output hoses, foot switch and pipette holder.

For precise and convenient movement of the electrode our three axes motorized micromanipulator and push button controller are included. This micromanipulator features hands free spatial resolution of 0.5 µm which enables positioning in the sub-micro range. Flexible motor coupling ensures no vibration of probe during movement.

The MB/B magnetic base provides a convenient position device for the micromanipulator.

Order #	Model	Product
W2 64-1608	PLS-1	Pico-Injector Micromanipulator System
W2 65-0002	PLI-100 Plus	Pico Injector
W2 60-0571		Right-handed motorized micromanipulator
W2 60-0577		Push button controller
W2 64-0060		MB/B Magnetic base

PLI-100

Medical Systems Pico-Injector

W2 65-0001 PLI-100 Pico-Injector

- 5 pressures: inject, balance, clear, fill and hold
- Reliable
- Femtoliter to microliter injections
- Reproducible performance
- Easy to use
- Popular applications:
  - Injection of mouse, frog, zebrafish and other oocytes
  - Extracellular brain injections
  - Injection of DNA, mRNA, microbeads, neurotransmitters, kinases and other proteins
- Most Published Injector

The **PLI-100 Pico-Injector** reliably delivers a wide range of volumes through micropipettes by applying a regulated pressure for a digitally set period of time. Compressed gas allows the user to deliver desired volumes from femtoliters to microliters while simultaneously holding a cell. Whether you need to do large injections into capillaries or very small injections into mammalian nuclei, the PLI-100 is well suited for your experiment.

The PLI-100 has become a favorite of prestigious national microinjection workshops like Cold Spring Harbor Laboratories and other researchers worldwide. Other companies have tried to design similar systems, but the PLI-100 remains unparalleled in terms of ease of use, durability, precision, and cost.

Researchers Say:

"The PLI-100 is very robust, in constant use in our lab."

"Most importantly, the PLI-100 valves prevent cytosol and yolk backflow into my pipette after oocyte injection."

"It's very easy to control."

"The PLI-100 is heavily used on a daily basis, and works great."

"I like the fact that I can use the PLI-100 with TTL pulses."

"It works great in conjunction with my imaging system."

"The balance pressure is a good option."

"My injection pipettes rarely clog."

Easy to Use

Inject with the touch of a button or a tap of the foot switch — it's as easy as that!

Reproducible

Pressure to the pipette is controlled precisely through a multi-turn regulator, and is reported digitally for easy repeat. Injection time is digitally controlled in 10 msec steps between 0.01 to 0.99 seconds (and in 1 second steps between 1 to 99 seconds). Pipette tip diameter, and hence delivered volume, are easy determinations once the timing and pressure are known.

Versatile

Deliver volumes from femtoliters to microliters with the same instrument, resulting in a wide range of applications.

Pressure Capabilities

The PLI-100 features two negative and three positive pressure pneumatic capabilities.

The negative, or vacuum functions allow the user to:

1. **Fill micropipettes from their tips, reducing wastage of valuable injectables.**
2. **Provide a means to secure and manipulate a cell using a holding pipette.**

Warner Instruments Inc. • Phone (203) 776-0664 • Toll Free U.S. (800) 599-4203 • Fax (203) 776-1278 • **www.warneronline.com**

PLI-100

Medical Systems Pico-Injector (continued)

The positive pressures allow the user to:

1. **Eject precise amounts of fluids.**
2. **Create a balance pressure which prevents backflow into the micropipette following an injection.**
3. **Clear a micropipette of material in it.**

Unique Features

The PLI-100's important 'Balance', 'Hold' and 'Clear' functions are not found on other microinjection units.

Balance

In addition to the ejection pressure, the Pico-Injector offers a secondary balance pressure. This secondary balance maintains a positive pressure on the injection pipette before and after injections. This eliminates dilution caused by capillary action and aids in the prevention of clogging. Wasteful continuous injection, which often occurs when no separate balance pressure is offered by an injection device, is avoided.

Fill/Hold

There are two built-in vacuum generators to fill a micropipette from the tip and to hold suspended cells. Filling the pipette from the tip is easier than back filling. Suspended cells can be held with a second (holding) pipette. The holding vacuum's range accommodates most cell types.

Clear

A high-pressure pulse can be used for clearing a pipette, should it happen to clog. This is particularly useful when working with pipettes sized for smaller volumes.

Electrical Connectors

BNC type connectors are available at the front panel to ease integrating the Pico-Injector with other equipment. Synchronization of injections to other stimulations or recordings is therefore possible.

Selection Guidelines

The PLI-100 is available in three packages: Plus, Basic and Deluxe. The basic unit is supplied with an input hose, output hose, holding hose, power cord and instruction manual. The plus unit also includes a foot switch, pipette holder and input hose adapter. The deluxe unit includes all the previously mentioned accessories plus an additional foot switch and one pipette holder.

Accessories

Available accessories for the PLI-100 Injection Systems are located on page 305.

Specifications

Input Gas Pressure	70 to 105 p.s.i. (480 to 720 kPa)
Injection Pressure	0.2 to 60 p.s.i. (413 kPa), regulated, multi-turn control
Balance Pressure	0.1 to 3.5 p.s.i. (68.9 kPa), regulated, multi-turn control, other ranges available upon request
Fill Vacuum	Internally produced, -12.0 p.s.i. (-82 kPa), unregulated
Holding Vacuum	Internally produced, 0 to 3 in H_2O (0 to 0.75 kPa or 0 to 0.1 p.s.i.), regulated
Clearing Pressure	Input gas pressure, unregulated
Injection Timer Pulse Width	0.01 to 0.99 sec in 10 msec steps; 1 to 99 sec in 1 sec steps
Injection Count Display	Digital, 0 through 9999
Duration Mode	Internally timed or externally gated
Time Trigger	Front panel, foot switch, or external TTL pulse (BNC)
Pressure Units	p.s.i./kPa; switch selectable
Pressure Monitor	BNC connector, 10 mV/p.s.i.
Pressure Readout	Inject, balance, clear, output port
Line Voltage	100/110/220/240 VAC
Power Usage	220 W
Meter Accuracy	0.1% full scale
Foot Switches	Inject, fill, hold, and gated; provided in plus and deluxe pkgs.
Weight	6.8 kg (15 lb)
Dimensions, H x W x D	11 x 38 x 25.5 cm (5 x 15 x 10 in)
Accessories Supplied	Input, output and holding hoses

Order #	Model	Product
W2 65-0001	PLI-100	PLI-100 Basic Pico Injector with Injection, Balance, Clear, Filling and Holding Pressures; Comes with Input Hose, Output Hose, Holding Hose, Power Cord and Instruction Manual
W2 65-0002	PLI-100 Plus	PLI-100 Plus Pico Injector with Injection, Balance, Clear, Filling and Holding Pressures; Comes with Input Hose, Output Hose, Holding Hose, Power Cord, Instruction Manual, Foot Switch, Pipette Holder and Input Hose Adapter
W2 65-0003	PLI-100 Deluxe	PLI-100 Deluxe Pico-Injector with Injection, Balance, Clear, Filling and Holding Pressures, Comes with Input Hose, Output Hose, Holding Hose, Power Cord, Instruction Manual, Two Foot Switches, Two Pipette Holders and Input Hose Adapter

PLI-90

Medical Systems Pico-Injector

W2 65-0004 PLI-90 Pico-Injector

- 3 pressures — inject, balance, and clearing
- Eliminates backflow into pipette after injection
- Reproducibly delivers femtoliters to microliters
- Easy to use
- Economical
- Precise

The **PLI-90 Pico-Injector**, like the reliable PLI-100 Pico-Injector, controls the precise and reproducible regulation of injection pressure and time.

Simplicity

Because the PLI-90 features only the injection, balance, and clearing pressures, it is a lower cost alternative to the PLI-100. This simplicity makes it even easier to use than the PLI-100.

Selection Guidelines

The PLI-90 is ideal for the user who does not require vacuum for filling pipette barrels or if using a holding pipette for holding cells is not essential to your application.

The PLI-90 is available in two packages: Basic and Plus. The basic model includes an input and output hose, handle, power cord and instruction manual. The plus model is supplied with all of the same parts as the basic model but also includes a Footswitch, Pipette Holder, and Input Hose Adapter.

Specifications

Input Gas Pressure	70 to 105 p.s.i. (480 to 720 kPa)
Injection Pressure	0.2 to 60 p.s.i. (413 kPa), regulated, multi-turn control
Balance Pressure	0.1 to 3.5 p.s.i. (68.9 kPa), regulated, multi-turn control, other ranges available upon request
Clearing Pressure	Input gas pressure, unregulated
Injection Time	0.01 to 0.99 sec in 10 msec steps; 1 to 99 sec in 1 sec steps
Pressure Display	Digital, three and a half digits
Duration Mode	Internally timed or externally triggered
Trigger Mode	Foot or panel switch
Pressure Readout	Inject, balance, clear, output port
Line Voltage	100/110/220/240 VAC
Power Usage	220 W
Foot Switch(es)	Optional inject and gating
Accessories Supplied	Input hose, output hose and power cord
Weight	6.8 kg (15 lb)
Dimensions, H x W x D	11 x 38 x 25.5 x cm (5 x 15 x 10 in)

Order #	Model	Product
W2 65-0004	PLI-90 BASIC	Pico-Injector with Injection, Balance and Clear Pressures; Includes Input Hose (PLI-IHN) and Output Hose (PLI-OHN), Handle, Power Cord and Inustruction Manual. Applications: Basic setups that do not need suction.
W2 65-0005	PLI-90 PLUS	Pico-Injector Basic Model and Acces-sories (Shown Above), Plus One Each PLI-FS Foot Switch, PLI-PH1 Pipette Holder and PLI-IHA Input Hose Adapter

PLI-100 and PLI-90

PLI-100 and PLI-90 Accessories

Order #	Model	Product
Accessories		
W2 65-0029	PLI-FS	Footswitch for Inject, Hold, Fill or Gate (Order more than one if frequent use of footswitch is needed for more than one of these functions.)
W2 65-0030	PLI-RM	Frame to Mount PLI-90 or PLI-100 in 19-in. Wide Instrument Rack
Hosing		
W2 65-0006	PLI-IHA	Input Hose Adapter (¼ in Male W2T Pipe Thread) Gas Bottle Regulator Fitting; Connects with PLI-IHO/N
W2 65-0007	PLI-IHO	Gas Input Hose (Tygon Tubing), 9 ft x 0.250 in (6.35 mm) x 0.125 in (3.18 mm) x 0.062 in (1.57 mm) (L x OD x ID x Wall Thickness); Connects to PLI-IHA and PLI 90/100 Gas Input, Brass Screw Fitting Type - Old
W2 65-0008	PLI-IHN	Gas Input Hose (Tygon Tubing) 9 ft L x 0.250 in (6.35 mm) OD x 0.125 in (3.18 mm) ID x 0.062 in (1.57 mm) Wall Thickness; Connects to PLI-IHA and PLI 90/100 Gas Input, Quick Connect/Disconnect Type - New
W2 65-0009	PLI-OHO	Output Hose (Tygon Tubing) 9 ft L x 0.071 in (1.80 mm) OD x 0.039 in (1 mm) ID x 0.016 in (0.41 mm) Wall Thickness; Connects to MSC Pipette Holders, Brass Screw Fitting Type - Old
W2 65-0010	PLI-OHN	Output Hose (Tygon Tubing) 9 ft L x 0.071 in (1.80 mm) OD x 0.039 in (1 mm) ID x 0.016 in (0.41 mm) Wall Thickness; Connects to MSC Pipette Holders and PLI 90/100 Gas Output, Quick Connect/Disconnect Type - New
W2 65-0011	PLI-HHO	Holding Hose with Cell Release Bulb; 9 ft L x 0.071 in (1.80 mm) OD x 0.039 in (1 mm) ID x 0.016 in (0.41 mm) Wall Thickness; Connects to MSC Pipette Holders and PLI-100 Hold Output, Brass Screw Fitting Type - Old
W2 65-0012	PLI-HHN	Holding Hose with Cell Release Bulb; 9 ft L x 0.071 in (1.80 mm) OD x 0.039 in (1 mm) ID x 0.016 in (0.41 mm) Wall Thickness. Connects to MSC Pipette Holders and PLI-100 Hold Output, Quick Connect/Disconnect Type - New

Order #	Model	Product
Pipette Holder/Adapter/Parts		
W2 65-0013	PLI-PH1	Stainless Steel Pipette Holder, 130 mm L for 1 to 1.5 mm OD Glass Pipettes
W2 65-0014	PLI-PH1A	Stainless Steel Pipette Holder, 80 mm L for 1 to 1.5 mm OD Glass Pipettes
W2 65-0017	PLI-SRG	Silicone Rubber Gasket Replacement for use with PLI-PH1 and PLI-PH1A, 10.2 cm (12 in)
W2 65-0015	PLI-SRG1.5	Silicone Rubber Gasket Replacement for use with 1.5 mm Glass Pipettes
W2 65-0018	PLI-SSB	Stainless Steel Bushing Replacement for use with PLI-PH1 and PLI-PH1A Pipette Holders
W2 65-0019	PLI-PC	Stainless Steel Pipette Cap Replacement for use with PLI-PH1 and PLI-PH1A Pipette Holders
W2 65-0020	PLI-HN	Stainless Steel Hose Nut Replacement for use with PLI-PH1 and PLI-PH1A Pipette Holders
W2 65-0021	PLI-PH-KIT	Pipette Holder Hardware Replacement Kit for use with PLI-PH1 and PLI-PH1A Pipette Holders, Includes 1 each PLI-SSB, PLI-PC, PLI-HN and PLI-SRG
W2 65-0022	PLI-PHA	Stainless Steel Pipette Holder (PLI-PH series) Adapter for Eppendorf ECET FEMTOTIP

Optional "Easy Insert" Acrylic Pipette Holder

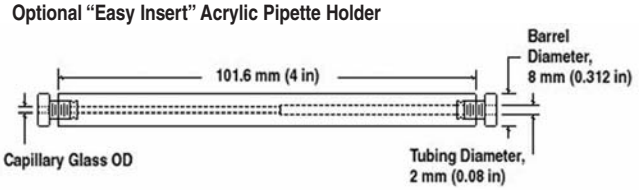

Order #	Model	Product
W2 69-0867	AO16 1.0	Acrylic Pipette Holder for 1.0 mm Pipettes
W2 69-0868	AO16 1.2	Acrylic Pipette Holder for 1.2 mm Pipettes
W2 65-0023	PLI-PPH	Acrylic Pipette Holder for 1.5 mm Pipettes
W2 69-0869	AO16 1.2	Acrylic Pipette Holder for 2 mm Pipettes

PM-8 and PM-4

8- and 4-Channel Pressure Injection Systems

W2 69-0153 8-Channel Pressure Injection System

- Multiple function system for micro-injection and perfusion
- Up to 8 injection/perfusion outputs, one hold cell output, and one synchronized drain out channel
- Programmable timers, counters, and step sequences which can be stored for reuse
- Manual control or automatic sequential step cycle operation
- Front panel display for pressures and programming information

The **PM-4** and **PM-8** programmable 4 and 8-Channel Pressure Injector Systems are designed for one to eight channel intracellular injection and extracellular perfusion. These microinjection and perfusion engines are especially designed for pharmacological drug testing, molecular biological DNA, RNA transferring, intracytoplasmic sperm injection and cell electrophysiological applications.

Combining an advanced micro-controller with precision pneumatic components, these systems can simultaneously control up to eight injection micropipettes or eight perfusion vials, one cell holding pipette, and one drain pipette. The four (PM-4) or eight (PM-8) injection/perfusion output ports can be controlled separately or combined together to perform actions such as injection, capillary action balancing, suction or clear up. The cell holding output port can produce an adjusted gentle suction to hold a cell, eject a pressure to push a cell, or completely clear the holding pipette. Another drain output port can simultaneously produce an adjusted suction to drain and clear out liquid before the next channel micro-perfusion. The PM-4/8 can deliver different quantity agents and drugs from picoliters to continuous perfusion. All output pressures and vacuums can be regulated and can be displayed real-time on the front panel display. Previous pressure readings can also be recovered on the display for setting comparison.

Besides programmable timers and counters, there are 16 programmable and savable injection/perfusion sequences with 32 programmable steps in each sequence. Each sequence can be repeated continuously or triggered manually. The interval time between steps can be programmed for automatic sequential cycle or manual trigger. There are two foot switch connectors for sequential step trigger and injection trigger. A digital remote port can be connected to an optional remote key pad or be controlled by a computer. With exceptional versatility and extremely precise control, either the PM-4 or 8 is an ideal multi-channel injection/perfusion engine.

Connection Diagram for Extracellular Micro-Perfusion and Intracellular Micro-Injection Systems

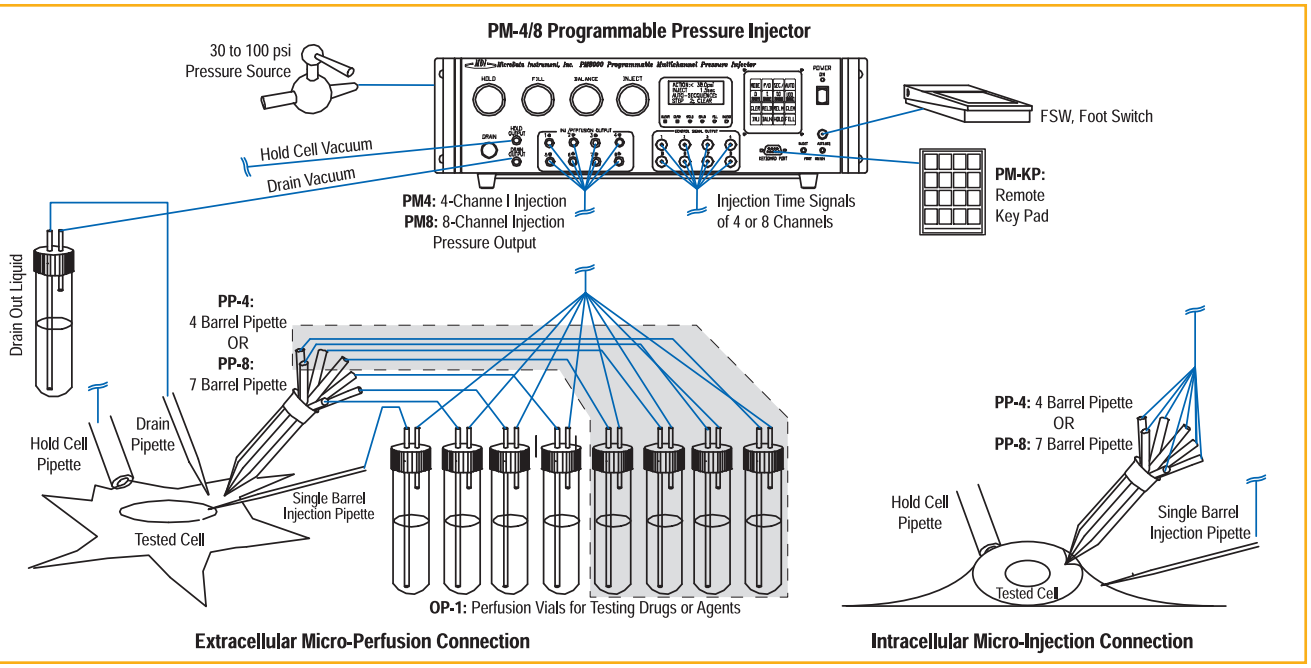
PM-4/8 Programmable Pressure Injector
30 to 100 psi Pressure Source
Hold Cell Vacuum
Drain Vacuum
PM4: 4-Channe l Injection
PM8: 8-Channel Injection
Pressure Output
Injection Time Signals of 4 or 8 Channels
FSW, Foot Switch
PM-KP: Remote Key Pad
Drain Out Liquid
PP-4: 4 Barrel Pipette OR PP-8: 7 Barrel Pipette
Hold Cell Pipette
Drain Pipette
Single Barrel Injection Pipette
Tested Cell
OP-1: Perfusion Vials for Testing Drugs or Agents
PP-4: 4 Barrel Pipette OR PP-8: 7 Barrel Pipette
Hold Cell Pipette
Single Barrel Injection Pipette
Tested Cell

Extracellular Micro-Perfusion Connection

Intracellular Micro-Injection Connection

Warner Instruments Inc. • Phone (203) 776-0664 • Toll Free U.S. (800) 599-4203 • Fax (203) 776-1278 • **www.warneronline.com**

PM-8 and PM-4

8- and 4-Channel Pressure Injection Systems (continued)

W2 69-0152 4-Channel Pressure Injection System

CE

Below are the components supplied with each of the **Pressure Injection Systems**.

Pressure Injection System		PM-4	PM-8
Order #	**Product**	**Qty.**	**Qty.**
W2 69-0154	IP1 Input Tubing with Connector	1	1
W2 69-0156	OP2 Output Tubing with Connector Only	6	10
W2 69-0157	FSW Foot Switch	1	1
W2 69-0164	PP-4 Pulled 4-Barrel Pipette	1	-
W2 69-0166	HOLD4 Holder for 4-Barrel Pipette	1	-
W2 69-0163	PP-7 Pulled 7-Barrel Pipette	-	1
W2 69-0167	HOLD7 Holder for 7-Barrel Pipette	-	1
-	Power Cord	1	1
-	User's Manual	1	1

Specifications

Output Channels	Four (PM-4) or eight (PM-8) injection / perfusion outputs, one synchronized drain out and one cell hold channel
Input Gas Pressure	30 to 100 p.s.i.
Clearing Pressure	Same as input pressure
Clear Hold Pressure	0 to 3 p.s.i. (regulated)
Injection Pressure	0.05 to 60 p.s.i. (regulated)
Balance Pressure	0.05 to 10 p.s.i. (regulated)
Fill Vacuum	0 to 24 in Hg (regulated)
Hold Vacuum	0 to 30 in of water (regulated)
Drain Vacuum	0 to 30 in of water (regulated)
Repeatability	±0.02 p.s.i.
Display Accuracy	±0.05 p.s.i. for pressure, ±0.2 in for vacuum (< 2 in H_2O)
Timer Setting Range	10 msec to 327.67 sec (10 msec resolution for whole range)
Counter Setting Range	1 to 255
Savable Sequences	16 sequences
Programmable Steps	32 steps for each sequence
Remote Control Ports	DB9 connector for remote key pad, foot switch jack and BNC for negative TTL trigger, jack connector for injection foot switch
Signal Output Ports	Eight BNCs for injection signal on output port 1 to 4
Power Consumption	100, 120 or 220 VAC, 35 W

Order #	Model	Product
W2 69-0152	PM-4	4-Channel Pressure Injection System
W2 69-0153	PM-8	8-Channel Pressure Injection System
Options and Accessories		
W2 69-0154	IP-1	Input Tubing with Connector
W2 69-0155	OP-1	Output Tubing with Connector and 4.5 ml Vial
W2 69-0156	OP-2	Output Tubing with Connector only
W2 69-0157	FSW	Footswitch
W2 69-0158	PM-KP	Remote Key Pad
W2 69-0160	RK-2	Rack Mounting Kit with Handles for PM 4/8
W2 69-0163	PP-7	Pulled Seven Barrel Pipette (each)
W2 69-0164	PP-4	Pulled Four Barrel Pipette (each)
W2 69-0165	HOLD-1	Holder for Single-Barrel Pipette
W2 69-0166	HOLD-4	Holder for Four-Barrel Pipette
W2 69-0167	HOLD-7	Holder for Seven-Barrel Pipette

W2 69-0156 Output Tubing with Connector for use with:
W2 69-0152, see above
W2 69-0153, see above
W2 69-0150, see page 223
W2 69-0151, see page 223

W2 69-0154 Input Tubing with Connector for use with:
W2 69-0152, see above
W2 69-0153, see above
W2 69-0150, see page 223
W2 69-0151, see page 223

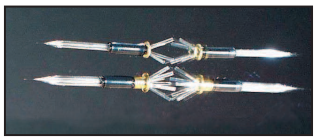

W2 69-0164 and **W2 69-0163** Pulled Pipettes for use with:
W2 69-0152, see above
W2 69-0153, see above

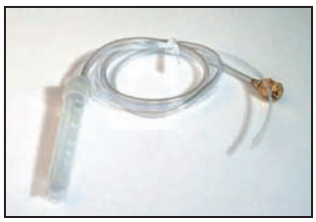

W2 69-0155 Output Tubing with Connector and 4.5 ml Vial for use with:
W2 69-0152, see above
W2 69-0153, see above
W2 69-0150, see page 223
W2 69-0151, see page 223

ZonaDrill™

Laser System

Use ZonaDrill™ for trouble free Cell Nuclear Transfer, ICSI and stem cell removal. ZonaDrill™ can also be used in conjunction with fluorescence.

Available with the Cronus software suite for cell/embryo analysis and digital target generator.

- High transmission optics for reduced laser pulse time
- Non-contact laser
- Mercury free Zona removal
- Digital display
- Easy to use and install

The New **ZonaDrill™** is a class 1 Laser System that incorporates the latest in fiber optic technology to provide the most compact laser system currently available. The ZonaDrill™ laser system is mounted via the epifluorescence port or side port of all popular brands of inverted microscopes. It can also be used in conjunction with all brands of micromanipulators and microscopes.

Rapid Zona removal is possible using the non-contact laser. Laser ablation is much faster than mechanical methods such as piezoelectric devices and manual micromanipulation. Improve your efficiency and effectiveness in the lab with this market leading product.

A visible wavelength pilot laser is used to target the main invisible ablation laser and the digital display informs the user when the laser is primed and ready to fire. The pulse duration of the laser is adjusted according to the hole size required. The digital display and compact hand control are unique features of this Laser system allowing easy and quick operation of the laser.

The latest ZonaDrill™ laser system incorporates a laser objective which provides a very high quality, high resolution image. It has also been designed for high transmission of the laser so that shorter pulse times are available to ablate the zona, resulting in increased embryo viability.

The ZonaDrill™ is the safest laser on the market and is guaranteed to be 100% accurate. The Unique Safety Circles, based on independent medical research, gives the user a visual indication of the Safety Zone for the protection of critical cells. This laser system features a unique hand-held control, a pilot laser targeting system and a digitally controlled pulse time. Additionally, the ZonaDrill™ requires no special needles/pipettes and is portable between microscopes.

Specifications

Ultra Focused Laser Beam:	
Solid State Diode Laser	1480 nm/300 mW
Power Density at Focus	4.5 mW/cm
Laser Focus Diameter	2 µm
Non-Mercury	
Pilot Laser	635 nm Spot Targeting Solid State Diode Laser
Objective Lens	40X

Order #	Product
W2 72-6475	ZonaDrill™ for Olympus IX50 / IX70
W2 72-6476	ZonaDrill™ for Olympus IX51 / IX71 / IX81
W2 72-6477	ZonaDrill™ for Nikon Eclipse TE 200/300
W2 72-6478	ZonaDrill™ for Nikon Eclipse TE 2000
W2 72-6479	ZonaDrill™ for Nikon Diaphot 200/300
W2 72-6480	ZonaDrill™ for Zeiss Axiovert 200
W2 72-6481	ZonaDrill™ for Zeiss Axiovert 100/135
W2 72-6482	ZonaDrill™ for Leica DMIRB

Nanoject II

Auto Nanoliter Injector

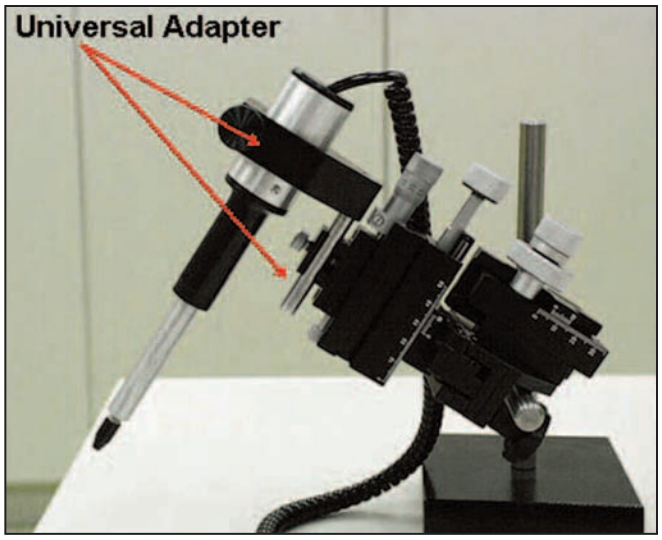

- Lower volume (2.3 nl) capability
- Positive displacement technology
- 2.3 to 69.0 nl range of volumes
- Minimal vibration
- New improved high torque motor
- Membrane key pad
- Improved micropipette holder
- Two speed injection/fill rates
- Auto 'Home' capability

The **Nanoject II** is the latest development in the Nanoject family of microinjectors. One unique features of the Nanoject II is the use of a high torque motor to provide smooth operation resulting in substantially reduced tip movement. A new collect configuration holds the micropipette more securely thereby reducing air infiltration and oil leakage. The two-speed fill/inject mode allows the user to fill and inject at half speed, facilitating the use of smaller micropipettes. The handling of more viscous samples is also improved. All of the above factors enhance the precise delivery of sample.

Volumes for the Nanoject II range from 2.3 nl to 69 nl. The smaller tips and smaller injection volumes of the Nanoject II allow users to perform injections into other specimens/applications that previously could not be performed.

Positive displacement technology and the use of precision micropipettes, eliminate the need for tedious calibration when the viscosity of the sample changes. Contaminants in the sample do not hinder or change the injection volume as with some other injectors. An optional universal mounting adapter provides easy mounting of the Nanoject II to a variety of micromanipulators and stereotaxic frames.

Specifications

Operation	Automatic
Glass Properties	Softening point 780°C
Glass Dimensions	1.14 x 0.053 mm (0.045 x 0.021 in) (OD x ID)
Injection Speed:	Fast: 46 nl/sec; Slow: 23 nl/sec
Fill Speed:	Fast: 46 nl/sec; Slow: 23 nl/sec
Empty Speed	92 nl/sec
Volume Range	2.3 nl to 69.0 nl
Change Volume	Dip switches #1 to #4
Change Inject Speed	Dip switch #5
Weight	99.2 g (3.5 oz)

Order #	Product
W2 69-0130	Nanoject II Nanoliter Injector, 115 V, 60 Hz, US Plug
W2 69-0131	Nanoject II Nanoliter Injector, 230 V, 50 Hz, European Plug
W2 69-0132	Nanoject II Nanoliter Injector, 230 V, 50 Hz, UK Plug
Replacement Parts	
W2 69-0133	Replacement Glass, 88.9 x 1.14 x 0.053 mm (3.5 x 0.045 x 0.021 in) (L x OD x ID), Vial of 100
W2 69-0134	Replacement Glass, 177.8 x 1.14 x 0.053 mm (7 x 0.045 x 0.021 in) (L x OD x ID), Vial of 100
W2 69-0135	Flared Glass, 90 mm (3.5 in), Vial of 100
W2 69-0136	Standard O-Ring
W2 69-0137	Special Flared O-Ring
W2 69-0138	Replacement Wire Plunger
W2 69-0139	Needle, 30 ga x 51 mm (2 in)
Accessories	
W2 69-0140	Footswitch
W2 69-0141	Support Base
W2 69-0142	Universal Mounting Adapter, see below photo

SLAM Soft Lipid-Assisted Microinjection Micropipettes

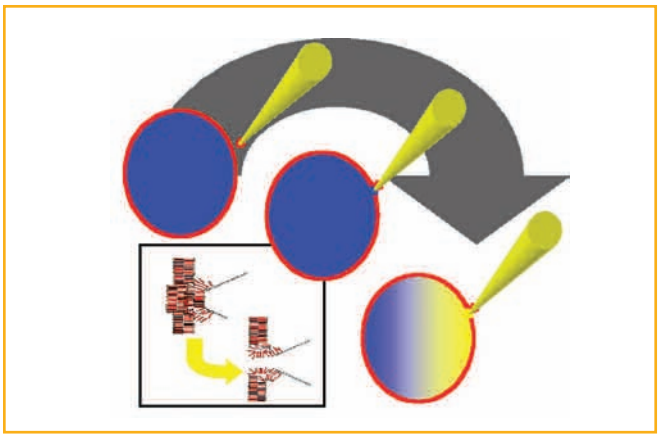

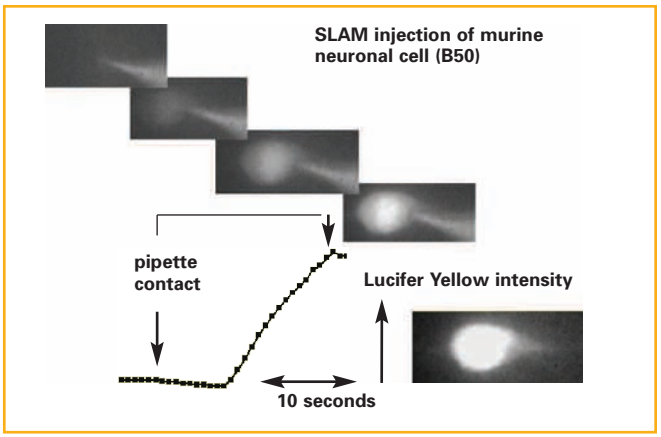

- SLAM – (Soft Lipid-Assisted Microinjection)
- An alternative to conventional microinjection. The glass micropipette does not penetrate the cell and there is no change in the pressure during injection.
- SLAM injection of neurones and other difficult cells
- Non-cell-penetrating

The tip of the glass micro-pipette is coated with a lipid bilayer to produce a non-cell-penetrating tip. Contact between the lipid bilayer at the micropipette tip and the cell membrane induces fusion between the respective lipid pools and an aqueous channel is formed between the inside of the micropipette and the cytosol.

Material to be injected, which is inside the micropipette, gains access to the inside of the cell either by diffusion or by low pressure ejection. In addition, the micropipette lipid transfers to the plasma membrane thereby permitting modification of the lipids in the plasma membrane by an entirely novel approach.

These techniques have been shown to work with a variety of cell types which are difficult or otherwise impossible to microinject.

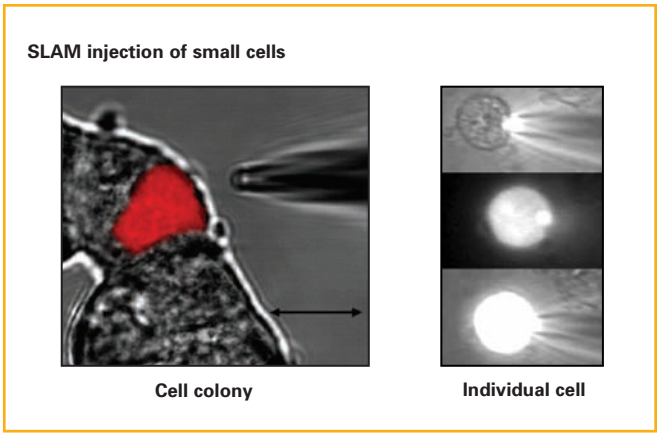

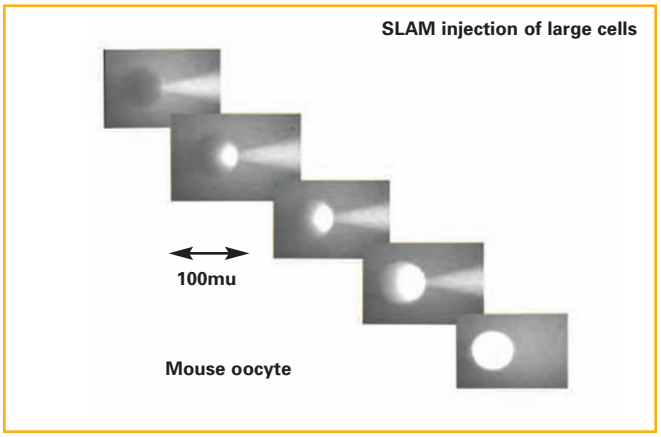

References

1. Laffafian and M. B. Hallett, Biophys. J. 75, 2558 (1998)

2. Peters RN, Sikorski R. The gentle slam. Science 282:2213-2214 (1998)

3. Carmichael SW. How to SLAM a cell. Microscopy Today 1999; 99/3:3

Order #	Model	Product
W2 64-1600	SLAM 05N	SLAM microinjection pipette, borosilicate, 0.5 µm tip
W2 64-1601	SLAM 10N	SLAM microinjection pipette, borosilicate, 1.0 µm tip
W2 64-1602	SLAM 05Q	SLAM microinjection pipette, quartz, 0.5 µm tip
W2 64-1603	SLAM 10Q	SLAM microinjection pipette, quartz, 1.0 µm tip

Micropipettes

Chemical Drilling Micropipettes

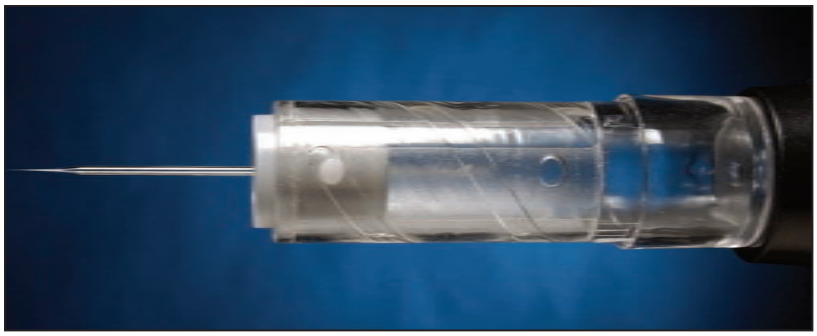

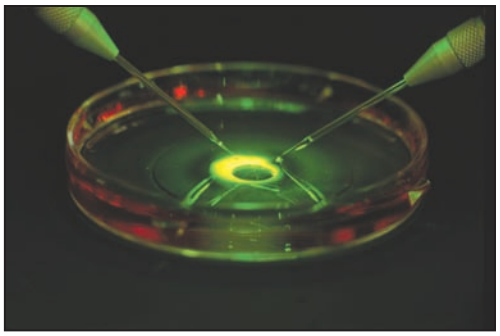

- Ideal for cell research
- Compatible with all micromanipulator systems
- Available in five bend angles
- Gamma irradiated sterilization
- Disposable

These **Micropipettes** are ideal for stem cell research. The Chemical Drilling Micropipettes are specially designed for use with PiezoDrills. These disposable Micropipettes are individually sterilized and available in five bend angles. They are manufactured in an independently validated clean room to FED.STD.209E, class 10,000. All processes are controlled to BSEN46002 and ISO 9002, resulting in ultra-clean and uniform micropipettes.

Each Micropipette is individually packed in a Twista-Pak™ that ensures easy, damage-free removal of the micropipette from its packaging. Five Twista-Paks are then sealed into a blister-pack to ensure that the micropipettes remain sterile and protected during freight.

Micropipettes, pkg. of 5

Bend Angle ID	Cell Holding Pipettes 15 µm	Cell Holding Pipettes 30 µm	Cell Removal Pipettes 20 µm	Cell Removal Pipettes 25 µm	Cell Removal Pipettes 30 µm	Cell Removal Pipettes 35 µm
0°	W2 72-6496	W2 72-6506	W2 72-7592	W2 72-7597	W2 72-7602	W2 72-7607
20°	W2 72-6497	W2 72-6507	W2 72-7593	W2 72-7598	W2 72-7603	W2 72-7608
25°	W2 72-6498	W2 72-6508	W2 72-7594	W2 72-7599	W2 72-7604	W2 72-7609
30°	W2 72-6499	W2 72-6509	W2 72-7595	W2 72-7600	W2 72-7605	W2 72-7610
35°	W2 72-6500	W2 72-6510	W2 72-7596	W2 72-7601	W2 72-7606	W2 72-7611

Bend Angle ID	Cell Injection Pipettes 5 µm	Cell Injection Pipettes 8 µm	Stem Cell Injection Pipettes 14-17 µm	Stem Cell Injection Pipettes 18-21 µm	Stem Cell Injection Pipettes 22-25 µm	Chemical Drilling Pipettes 10 µm
0°	W2 72-7582	W2 72-7587	W2 72-6486	W2 72-6511	W2 72-6491	W2 72-6501
20°	W2 72-7583	W2 72-7588	W2 72-6487	W2 72-6512	W2 72-6492	W2 72-6502
25°	W2 72-7584	W2 72-7589	W2 72-6488	W2 72-6513	W2 72-6493	W2 72-6503
30°	W2 72-7585	W2 72-7590	W2 72-6489	W2 72-6514	W2 72-6494	W2 72-6504
35°	W2 72-7586	W2 72-7591	W2 72-6490	W2 72-6515	W2 72-6495	W2 72-6505

Screw-Actuated Syringes

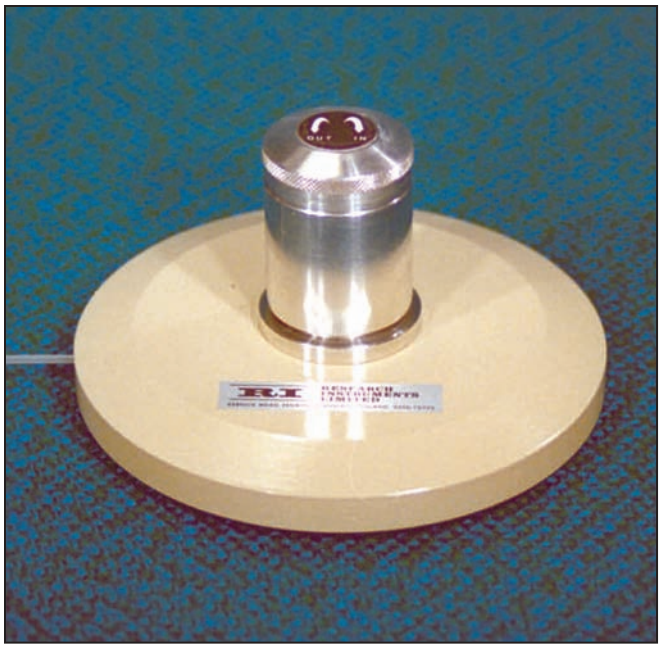

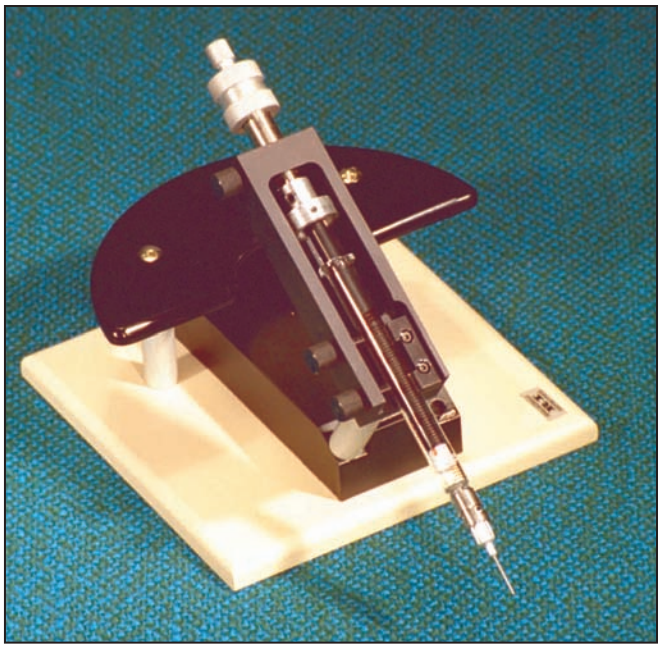

- For air-assisted microinjection and microaspiration
- Uncomplicated and easy to use
- Accurate
- Sensitive control
- High suction/pressure

Screw-Actuated Air Syringes

These air-assisted microinjection/microaspiration syringes provide the user with sensitive control and an extremely low dead-air volume. The capacity of the syringe is 10 ml. When required, the syringes can be used to generate high pressure or suction.

The **Screw-Actuated Syringe** is a small compact unit incorporated into a heavy circular base. Its convenient dimensions enable it to be ergonomically positioned next to the control lever of a micromanipulator to facilitate single-handed operation of both instruments.

The syringe is connected by hard polyethylene tubing to a micropipette, which in turn, may be fitted to a micromanipulator or positioning device. Suction/injection is obtained by turning the metal colored actuator screw-control on the top of the syringe. The syringe provides a solution to the problem of capillary action when working with small micropipettes. A small balance (equilibrating) pressure can be maintained to offset the effects of capillary action. A conveniently situated release-button on-top of the screw-control is provided to achieve equilibration.

Order #	Product
W2 69-0105	Screw-Actuated Air Syringe

- Ideal for oil-filled injection/aspiration
- Easy to use
- Hamilton syringe incorporated
- Accurate
- Sensitive control
- Low dead-air volume
- High suction/pressure
- Easy to exchange or replace the syringe

Screw-Actuated Micrometer Driven Hamilton Syringe

This screw actuated syringe is a micrometer-actuated syringe mechanism mounted on a small base. This syringe is for oil/air-assisted micro-injections and micro-aspirations. Its compact dimensions enable it to be ergonomically positioned next to the control lever of a micromanipulator to facilitate single-handed operation of both instruments.

Suction/injection is achieved by using the rotary-actuator with a fine micrometer-thread, which has a 15 mm movement range. A 1 ml gastight Hamilton glass syringe with a Luer-taper is incorporated. A Luer-taper hypodermic needle is mounted on the taper of the Hamilton syringe. The syringe is connected by hard polyethylene tubing to a micropipette, which in turn, may be fitted to a micromanipulator or similar instrument. The 1 ml Hamilton syringe can be easily exchanged for any other Hamilton 1700 syringe series including the 1000, 500, 200, 100 and 50 µl sizes, visit www.harvardapparatus.com for complete details.

Order #	Product
W2 69-0107	Screw-Actuated Micrometer Driven Hamilton Syringe

Warner Instruments Inc. • Phone (203) 776-0664 • Toll Free U.S. (800) 599-4203 • Fax (203) 776-1278 • **www.warneronline.com**

Vibratome®

Tissue Sectioning Systems

W2 69-0353
Vibratome® 1000 Classic

- The world standard for tissue sectioning systems for 30+ years
- Cuts fresh or fixed tissues without distortion
- Patented vibrating blade principal
- Sections as thin as 6 µm (using sapphire blade)
- Less damage than oscillating blade systems
- Automatic and refrigerated models available
- Simple and quiet operation
- Easily maintained
- Secure specimen holding vice
- Stable blade holder insures no unintentional setting changes
- Cool lamp magnifier — minimizes heating effect and provide shadow-free illumination

The Vibratome® series of fresh tissue sectioning systems allows sectioning of fresh or fixed tissue without freezing or embedding. The patented vibrating blade principle moves the sectioning blade edge in a reciprocating arcuate path as it penetrates the specimen. The reduced effective edge angle from the transverse movements, with the lateral distribution of the cutting edge penetrating pressure, minimize elastic deformation of soft tissue specimens that are simply held or capsulated in position during the sectioning operation.

Uniform sections can be made of delicate soft, tissue specimens. Sections are free of observable compressive distortion in the direction of cut, as would be typical with conventional microtomes using oscillating blade actions. Preservation of ultrastructure is maintained in the sections from a lack of cellular damage on their surfaces. Sectioning takes place in a liquid bath. The liquid serves to lubricate the sectioning blade, to maintain specimen temperature, enhance or preserve desirable characteristics of the specimen, and facilitate the easy retrieval of the sections generated.

Using the technique described, the Vibratome® series of microtomes deliver superior performance using ordinary injector type razor blades. Sectioning of uniform fresh tissue sections can be cut from 20 µm up, although thinner sections may be realized, depending on the type of tissue involved, and operator technique. For conventional use, expensive blades made from exotic materials are not required, cutting the costs of normal operation and maintenance. If a more precise and finer tissue slice is required, use a sapphire blade which provides slices as thin as 6 µm. All Vibratomes® can work with standard, glass, sapphire or injector knife holders.

Typical applications include: Enzyme histochemistry, tissue pathology, autoradiology, water soluble compounds, immunocytochemistry, immunohistochemistry, fluorescent microscopy, tissue pathology, botanical studies, preparation step prior to Electron Microscopy, invaluable teaching aid, etc. Five different Vibratomes® available to fit your applications and your budget.

Vibratome® 1000 Classic

The original Vibratome® semi-automatic fresh or fixed tissue sectioning system has maintained a long reputation as a rock solid tissue sectioning system. Researchers from around the globe have relied on the Vibratome® 1000 Classic for their fresh tissue sectioning needs for over 30 years.

Vibratome® 1000 Plus

The Vibratome® 1000 Plus utilizes the same mechanical sectioning components with enhanced specifications and features such as: smaller section thickness increments, increased sectioning speed, faster return stroke speed, increased maximum sectioning range, drain function, standard dual bath, and finer height adjustment. A stroke pause switch and adjustable light and magnifier are also part of the Vibratome® 1000 Plus system. The Vibratome® 1000 Plus is a solid addition to the Vibratome® family of products.

Vibratome® 3000 Plus

The Vibratome® 3000 Plus sectioning system provides a versatile means of sectioning fresh or fixed, animal, or plant tissues. This system employs a vibrating blade principle which allows sectioning without freezing or embedding. The creation of artifacts, the alteration of morphology, the destruction of enzyme activities, and other deleterious effect inherent in freezing or embedding procedures are thus avoided. The Vibratome® 3000 Plus incorporates a full english text display for added ease and usability. The 3000 Plus utilizes the Vibratome® Companies "ZERO-Z" Technology which dramatically reduced z-axis vibrations. This system also has a dynamic stability system and deluxe bath system as standard. The Vibratome® 3000 Plus provides the best quality section in the Vibratome® product line.

Vibratome® 3000 Deluxe

The Vibratome® 3000 Deluxe includes all the enhanced features of the 3000 Plus sectioning system plus a built in thermoelectric cooling device for the specimen bath. The refrigeration is a great benefit for those researchers trying to maintain constant temperature and constant chemical makeup of buffer solution.

Vibratome®

Tissue Sectioning Systems (continued)

CE

Vibratome® 3000

Vibratome® 1500

The **Vibratome® 1500** is the newest member of the Vibratome® family and features a fully automatic tissue sectioning system. Users can simply enter the number of sections and thickness required and the Vibratome® 1500 does the rest. Through the use of an easy to read LED display and simple controls, the Vibratome® 1500 makes serial sectioning an easy task.

All Vibratomes® are supplied complete with: Blade Angle Indicator, Vice-Type Specimen Holder, Specimen Mounting Blocks, Bath (146 x 146 x 50 mm, 5.75 x 5.75 x 2 in), Black Buffer Bath, Dust Cover, Magnifying Lamp, Fluorescent Tube, Specimen Adhesive, Razor Blades, Spare Fuse and Operating Instructions. All Vibratomes® have an Adjustable Specimen Angle Range of 0-50 degrees and can be used with Standard, Glass, Sapphire or Injector Knife Holders. **Other optional accessories include:** Rotating Stage Assembly, Specimen Mounts, V-Block Adapter, Section Mounting Device, Specimen Tray, Sapphire Knife, Glass Knife Adapter and Specimen Retrievers.

Specifications

	Vibratome® 1000 Classic	Vibratome® 1000 Plus	Vibratome® 1500	Vibratome® 3000 Plus	Vibratome® 3000 Deluxe
New Zero Z Technology	No	No	No	Yes	Yes
Adjustable Frequency*	No	No	No	Yes	Yes
Dynamic Stability System	No	No	No	Yes	Yes
Total Vertical Specimen Stroke	10 mm	15 mm	15 mm	15 mm	15 mm
Adjustable Sectioning Window	No	Yes	Yes	Yes	Yes
Section Thickness Increments	10 µm	5 µm	5 µm	5 µm	5 µm
Maximum Specimen Size	25 x 25 x 10 mm	60 x 40 x 15 mm	60 x 40 x 15 mm	60 x 40 x 15 mm	60 x 40 x 15 mm
Sectioning Speed	0 - 1.25 mm/s	0 - 5 mm/s adjustable	0 - 5 mm/s adjustable	0 - 5 mm/s adjustable	0 - 5 mm/s adjustable
Return Stroke Speed	1.25 mm/s	5.0 mm/s max	5.0 mm/s max	5.0 mm/s max	5.0 mm/s max
Maximum Sectioning Range	30 mm	40 mm	40 mm	40 mm	40 mm
Drain	No	Yes	Yes	Yes	Yes
New Deluxe Dual Bath System	Optional	Optional	Optional	Standard	Standard
Multi Specimen Sectioning	Optional	Optional	Optional	Standard	Standard
Repeatable Height Adjustment	10 µm	5 µm	5 µm	1 µm	1 µm
Use Disposable Microtome Blades	Yes	Yes	Yes	Yes	Yes
Rotating Specimen Mount	Yes	Yes	Yes	Yes	Yes
Stroke Pause Switch	No	Yes	Yes	Yes	Yes
Separately Adjustable Light and Magnifier	No	Yes	Yes	Yes	Yes
Arcuate Blade Path Adjustment	Yes - 1.25 mm	Yes - 1.5 mm	Yes - 1.5 mm	Yes - 2.0 mm	Yes - 2.0 mm
Foot Switch	No	Optional	Optional	Standard	Standard
Fully Automatic Operation	No	No	Yes	Yes	Yes
Insulated Bath	No	Yes	Yes	Yes	Yes
Built In Refrigeration	Optional	Optional	Optional	Optional	Standard
Cumulative Section Counter	No	No	No	Yes	Yes
Full Text LCD Display	No	No	No	Yes	Yes
0.01 Increment Sections	No	No	No	Yes	Yes
Specimen Auto-Bypass	No	No	No	Yes	Yes
110 VAC	**W2 69-0353**	**W2 69-0350**	**W2 69-0446**	**W2 69-0442**	**W2 69-0444**
220/230/240 VAC	**W2 69-0354**	**W2 69-0351**	**W2 69-0447**	**W2 69-0443**	**W2 69-0445**

** Zero Z technology includes an adjustable frequency mode*

Warner Instruments Inc. • Phone (203) 776-0664 • Toll Free U.S. (800) 599-4203 • Fax (203) 776-1278 • **www.warneronline.com**

Vibratome®

Tissue Sectioning System Accessories

Order #	Product
W2 69-0368	Replacement Fluorescent Tube
W2 69-0376	Specimen Adhesive, 1/3 oz. Bottle
W2 69-0377	Blade, Single Edge Injector, pkg. of 10

Vibratome® Care Package

Order #	Product
W2 69-0382	The Vibratome® Care Package; Includes 10 Vibratome® Feather Blades, 1 bottle of Specimen Adhesive, 3 Specimen Mounting Blocks, a Specimen Tray, 2 fuses and 1 Spare Fluorescent Bulb.

Vibratome® The Works

Order #	Product
W2 69-0383	The Works; Includes everything from the Vibratome® Care Package plus Rotating Stage, 0.5 inch Specimen Mounts, Replacement Rotating Mounts, Storage Block, Specimen Retrievers, and Section Mounting Device

Listed below and to the right are optional accessories to the Vibratome Tissue Sectioning System. Select your options based on your tissue slicing requirements

Sapphire Knife

This sapphire microtomy knife makes it possible for the first time to cut thin Vibratome® sections with microscopic resolution similar to that obtained with thick 1 µm plastic sections. The sapphire knife allows routine serial sectioning with a Vibratome® 1000 Plus of a thickness in the 6 to 10 µm range, revealing sub-cellular features never before seen. With a Vibratome® 3000, sections of mildly fixed tissue as thin as 2 µm may be obtained. The sapphire knife can be re-sharpened.

Order #	Product
W2 69-0378	Sapphire Knife

Specimen Mounting Blocks

These Specimen Blocks are utilized for mounting specimens and placing in the Vibratome® holding vice. The blocks are annodized black for easy specimen viewing and can be reused.

Order #	Product
W2 69-0370	Specimen Mounting Block

Specimen Mounts 1⁄2 inch Head

Specimen mounts are designed to allow for the rotation of the specimen in the Vibratome® vice assembly for sectioning at different horizontal orientations.

Order #	Product
W2 69-0372	Specimen Mount 1⁄2 inch Head

Specimen Retriever

This is a perfect tool for retrieving free floating sections from the bath.

Order #	Product
W2 69-0380	Specimen Retrievers, pkg. of 5

V-Block Adapter

Adapter for holding special specimen mounts in the Vibratome® vice, black anodized.

Order #	Product
W2 69-0371	V-Block Adapter

Section Mounting Device

A simple device designed to mount floated histological sections onto standard glass slides. This product facilitates the mounting of all types of thin (2 µm to 100 µm) tissue slices. It is especially useful for mounting tissue slices not supported by embedding material, such as those produced with a Vibratome®, freezing microtome (cryostat) or sliding microtome. It also simplifies the mounting of tissue sections embedded in a water-miscible supporting medium such as polyethylene glycol (PEG).

Order #	Product
W2 69-0381	Section Mounting Device

Specimen Tray

This tray holds the tissue in an appropriate buffer. Replaces the standard mounting block. Surrounded by ice in the bath, it will keep the buffer cold without disturbing the sections. The tray saves buffer, allows easier clean up and keeps contamination to a minimum. A rectangular projection on the bottom of the tray fits directly into the specimen vice. Inside dimensions 76 x 55 x 9.5 mm (3 x 2.1875 x 9.375 in).

Order #	Product
W2 69-0369	Specimen Tray

Deluxe Specimen Bath

The Deluxe Specimen Bath mounts inside the existing black Vibratome® bath. This large removable bath allows for the separation of buffer and ice kept in the original black bath. The Bath can be sterilized and has round mounting disks that can be easily removed for mounting specimens. The disks and bath surface are marked with degrees of rotation for the repeatable placement and measurement of specimens.

Order #	Product
W2 69-0440	Deluxe Specimen Bath

Glass Knife Adapter

The glass knife adapter allows you to routinely cut 20 µm sections of fresh tissue and even thinner sections of fixed tissue. Simply replace the standard razor blade holder with our special glass knife adapter and use ordinary 1 in-wide glass knives. The entire assembly is black anodized aluminum.

Order #	Product
W2 69-0379	Glass Knife Adapter

Rotating Stage Assembly

This assembly allows a specimen to be oriented to the blade after it has been affixed to the specimen mount. At a 20° blade angle, the rotating stage assembly will adjust up to 15°, still allowing 10 mm clearance. Replaces the standard Vibratome® vice assembly. Everything is black anodized aluminum.

Order #	Product
W2 69-0373	Rotating Stage Assembly

EMS 4000

Automatic Oscillating Tissue Slicer

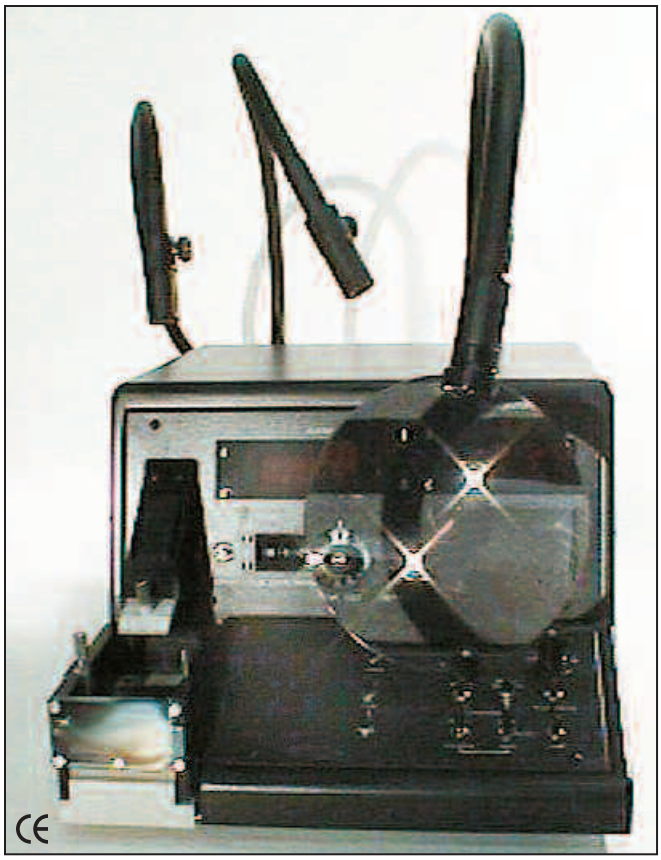

- Automated functions dramatically reduce preparation time by eliminating the need for embedding or freezing your sample
- Eliminates the risk of distortion and artifacts associated with embedding and freezing
- Provides consistent slices as thin as 10 µm
- Optional built-in refrigeration maintains temperature during slicing for maximum tissue life

Features

- **Slice thickness set in 10 µm increments on thumbwheel: push button advance; digital display status**
- **New ultra light blade oscillation mechanism mounted on heavily reinforced chassis minimizes vibration**
- **Linear cutting blade motion to 4000 CPM**
- **Blade mechanism above bath simplifies maintenance; easy to clean, removable tray**
- **Motorized variable speed specimen advance; momentary or continuous modes**
- **Auto-sectioning controls permit consecutive sections to be cut automatically**
- **Available with integral refrigeration system**
- **Pure white, high intensity halogen lamp with fiber optic light pipes and diffusing lens**
- **Blade activation can be achieved through 2-position toggle switch for continuous cutting action or with removable foot pedal**
- **Mounting of specimen can be done directly on unique tissue pedestal with option of using pivot pin or just setting pedestal flat on bottom of tray on 90° angle. In addition, sample vice holder (with pivot pin) can be attached to tray and mounting blocks when used. Both devices come standard with unit.**
- **Adjustable blade angle indicator is built into arm of unit**
- **X2 magnifying lens (4 in. D) included**
- **Optional glass knife holder is available to hold 6.4 x 25 mm glass knives**

The **EMS 4000** Oscillating Tissue Slicer represents the solution to sectioning either fixed or fresh tissue. There is no need for embedding or freezing your sample, so preparation time is dramatically reduced. The risk of distortion and artifacts, normally associated with these procedures, are therefore eliminated.

This tissue slicer has an ultra light blade mechanism, which is mounted on a heavy reinforced chassis reducing any effects from vibration. For exacting precision, the EMS 4000 has a thumb-wheel switch to select the thickness as well as automatic control circuitry so that consecutive sections may be cut easily and rapidly. The unit also features motorized control of the blade height and a complete digital display of the total cutting excursion. The blade speed and the motorized specimen advance controls are precisely controlled by a variable speed adjustment. The blade advance may be set to either a continuous mode or a momentary advance toggle switch. The specimen-collecting tray is removable and easy to clean. All controls may be set with one hand and there are options for manual or automatic cutting of pre-selected cutting thicknesses. The optional refrigeration unit will maintain the tray temperature near 0°C during the sectioning process to offer maximum tissue life and best cutting consistency. A tap water flow of 250 ml per minute is required during operation. The solution in the tray is cooled directly so there is no vibration associated with the cooling aspect of the unit.

The unit comes complete with a 20 watt halogen white light lamp with dual fiber optic light pipes and diffusion lens, a magnifying lens mounted on flexible goosenecks and a media tray with a clear front tray panel to allow for maximum sample exposure. As well, complete with the unit comes a tissue pedestal, specimen vice holder, and specimen blocks. The media tray, which measures 95 x 25 x 48 mm (larger size available as an option) requires minimal amount of buffer and is made from a single block of Delrin. The tissue pedestal, with pivotal pin, allows you to mount your specimen directly to the pedestal and to change the angle of your specimen relative to the blade, hence offering you perfect specimen orientation. The sample vice holder (with pivotal pin) allows you to adhere your specimen directly to a mounting block. A glass knife holder is available as an option for the mounting and cutting with glass knives. The EMS 4000 meets the highest standards for precision and accuracy and it matches the performance of units on the market costing twice as much.

Warner Instruments Inc. • Phone (203) 776-0664 • Toll Free U.S. (800) 599-4203 • Fax (203) 776-1278 • **www.warneronline.com**

EMS 4000

Automatic Oscillating Tissue Slicer (continued)

Specifications

Tissue Slicer Controls

Blade Advance, Direction	2-position toggle switch for selecting advance or return blade motion
Blade Advance, Mode	3-position toggle switch (center off) for selecting continuous advance at selected rate or momentary advance when 'spring-back' toggle is depressed
Manual/Auto Mode	2-position toggle switch, in manual position, blade drive stops at end of its forward or reverse travel, in auto mode, blade will automatically reverse direction at its maximum forward position (or when change direction push button is activated), return to maximum reverse position, activate slice thickness increment, and begin forward cutting sequence
Change Direction	Push button (for use in auto mode) which reverses blade direction when tray is advancing. Control permits operator to save time that would be used to complete forward cycle after section is cut.
Blade Advance, Rate	1-turn potentiometer with calibrated dial for selecting rate of blade advance (tray return rate is always 2.0 mm per sec.)
Blade Position, Direction	2-position toggle switch for selecting up or down motion
Blade Position, Mode	2-position switch for selecting continuous or single steps
Blade Height, Step	Push button switch for initiating single step equal to slice thickness selected on thumbwheel switches
Blade Height, Reference	Push button switch to zero 5-digit LED display
Slice Thickness	3-digit thumbwheel switches for selecting slice thickness in 10 micron increments (least significant digit on 3-digit bank is fixed at 0)
Blade Oscillation Speed	1-turn potentiometer with calibrated dial for selecting blade speed from 60 to 4,000 cpm
Oscillating Blade Motion	2-position toggle switch for selecting motion continuously on or activation by foot switch on 2 m (6 ft) cord
Power	2-position rocker switch for activating line voltage
Temperature Set	1-turn potentiometer with calibrated dial proportional to temperature selected W2 69-0251 only
Refrigeration	2-position toggle switch for activating refrigeration unit W2 69-0251 only

EMS-4000 Oscillating Tissue Slicer

Blade Height Adjustment	35 mm total travel adjustable in 10 µm increments set on digital thumbwheel switches
Slice Thickness	Adjustable from 10 to 990 µm in 10 µm increments
Blade Speed	Continuously adjustable from 60 to 4,000 cycles/min
Blade Oscillation Amplitude	Linear, 1.2 mm traverse (other lengths optional)
Blade Angle	Adjustable from 5 to 30° C
Blade Advance:	
Travel	31 mm total
Forward Speed	Continuously adjustable from 0.1 to 2.0 mm/sec
Reverse Speed	2 mm/sec
Specimen Size	15 x 25 x 25 mm (0.6 x 1.0 x 1.0 in) max volume, H x W x D
Lamp	20 W halogen white lamp with dual fiber optic light pipes and diffusion lens on 46 cm (18 in) gooseneck
Magnifier	10 cm (4 in) D X2 lens mounted on 30 cm (12 in) gooseneck, 22.9 cm (9 in) working distance
Temperature Range	(80-15-1-02 only) 0°C to ambient, temperature displayed on 3-digit LED to 1°C

Specifications (continued)

Dimensions	18 x 27 x 40 cm (7.5 x 10.5 x 16 in), H x W x D
Weight	13 kg (30 lb)
Working Space Requirements	25 x 30 x 46 cm (10 x 12 x 18 in), H x W x D
Power	115/230 VAC, switch selectable, 50/60 Hz
Certification	CE marked

This tissue slicer is supplied complete with media tray, tissue pedestal, sample vice holder, 25 blades, dust cover, 3 anodized aluminum blocks, foot switch, lamp and 2 fiber optic light pipes, magnifying lens, adhesive, and operating instructions.

Order #	Product
W2 69-0250	EMS-4000 Oscillating Tissue Slicer
W2 69-0251	EMS-4000 Oscillating Tissue Slicer with Built-In Refrigeration
W2 69-0252	Refrigeration Retrofit
W2 69-0253	Replacement Bulb
W2 69-0254	Replacement General Purpose Razor Blades, pkg. of 25
W2 69-0255	Replacement Tissue Pedestal for Standard Tray
W2 69-0256	Replacement Tissue Pedestal for Large Tray
W2 69-0257	Replacement Adhesive, pkg. of 5
W2 69-0258	Glass Knife Holder, Allows Reproducibly Cut Fresh (10 µm Sections) and Fixed Tissues; Attaches Directly to Unit and Accommodates 6.4 x 25 mm (0.25 x 1 in) Glass Knives
W2 69-0259	Large Media Tray with Pedestal, 95 x 25 x 73 mm (3.7 x 1 x 2.9 in) (Internal Dimensions)
W2 69-0260	Histology Glass Knife Strips, 6.4 x 25 x 400 mm (0.25 x 1 x 15.75 in), pkg. of 30
W2 65-0076	BSC-PC Pre-Chamber; Allows 10 to 12 Brain Slices to be stored in vitro for several hours while maintaining excellent viability. Mixture of 95% O_2/5% CO_2 is bubbled through physiological saline, to initiate circular flow and oxygen enriched saline, which continuously permeates slices. Slices remain viable for hours while awaiting transfer to examining chamber.
W2 69-0262	Slicer Kit; Assists when using Oscillating Tissue Slicer; Kit includes Sable Brush, Parafilm 4 x 250 ft, Quick Bond (pkg. of 5 Tubes), Kimwipes, pair of Tweezers (#5, #6, #7), Fontax, Specimen Forceps (4 and 6 in.), Six 8 ml Sample Specimen Bottles with Caps, Six 5 ml Glass Micro-Beakers, Six 7.5 ml Glass Microbeakers

McIlwain

Mechanical Tissue Chopper

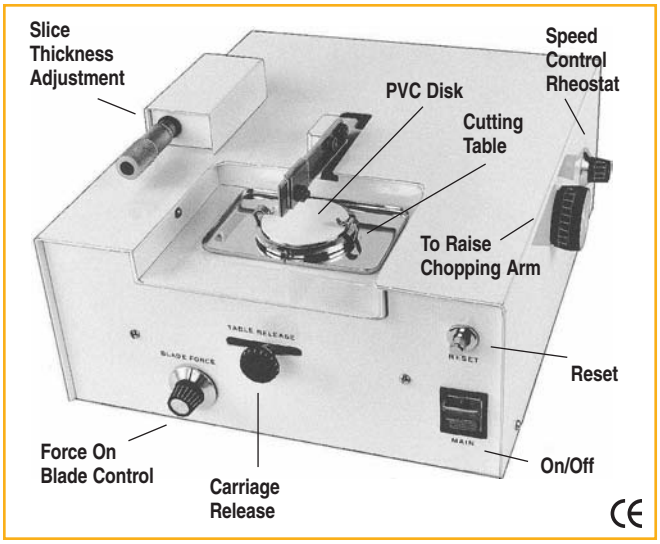

- Less disturbance of cell structure than homogenizers or blenders
- Slices up to 1 mm thick and cubes or prisms up to 1 mm cross section
- Designed to prepare tissue for metabolic experiments

This **McIlwain** tissue chopper has been designed to prepare pieces of tissue for metabolic experiments. It is especially suited for small and irregular specimens from biopsy or small organs. The Tissue Chopper causes much less disturbance of the cell structure than homogenizers or blenders, and is applicable to fragments which would be difficult or impossible to cut. It has been applied to liver, kidney and various parts of the central nervous system.

This tissue chopper will produce slices up to 1 mm thick Cubes or prisms up to 1 mm in cross section can also be prepared within 30 seconds. The stepless variation of slice thickness from zero to the maximum is controlled by an index clutch in conjunction with a micrometer head. The latter being calibrated in microns.

The action of the machine is as follows: a circular stainless steel table, on which the specimen is placed, is traversed from left to right at a speed which can be varied. At the same time a chopping arm carrying a blade is raised and dropped by its own weight and the tension of a spring, at speeds varying from zero to a maximum of 200 strokes per minute. As the table carrying the tissue passes under the blade it is chopped into the required slices. If prisms are required the table is returned to the left hand side of the machine, turned through 45 degrees, and the process repeated. Cubes are formed by rotating the table 90 degrees. A safety limit switch is provided to prevent the machine overrunning and a quick return mechanism is fitted for the return of the table. All parts coming into contact with the tissues are of stainless steel. Finish is in white powder coat.

Note: The above description is extracted from an article by H. McIlwain and H. L. Buddle in the Biochemical Journal, Vol. 53, No. 3, pp. 412–420, 1953, by their permission.

Operation

1. Positioning Blade: Filter papers are placed on the circular table and a blade loosely clamped to the arm. The arm is brought to rest on the stop rod by rotating the handwheel on the motor shaft and the blade pressed down with the fingers. The blade is then securely clamped in this position. The machine is switched on and it will probably cut the top filter paper. This is removed and the machine is ready to take a specimen.
2. Slice Thickness: The thickness of slice is adjusted by means of the micrometer head. The maximum thickness is 1 mm. Each division on the thimble is 1 µ. Each small division on the barrel is 25 µ.
3. Force on Blade: The force on the cutting arm can be adjusted by the front knob. To increase tension turn in clockwise direction.
4. Cutting: Pull out the carriage release knob and slide the table to the left of the machine. Place the specimen on the centre of the table and with the rheostat in the slow position switch on the bottom switch. Increase the rheostat until the desired speed has been attained. After the tissue has been cut into slices it may, if desired, be turned 90 degrees and formed into cubes, after passing under the cutting arm again. The machine automatically switches itself off at the end of its travel. When this limit switch is used it must be reset by means of the top button. The cutting arm is made of stainless steel and may be removed for the purpose of sterilization.
5. Plastic Cushion: This machine is now fitted with a plastic cushion held in place by two spring clips on the table. The specimen may be fixed to a suitable filter paper by means of a fixative such as agar, which in turn is cemented to the cushion, and then inserted under the springs. This arrangement holds the specimen firmly down and prevents it sticking to the blade during chopping.

Specifications

Maximum Blade Height	~1 cm
Slice Thickness Settings	1 mm maximum with 1 mm scale resolution
Minimum Section Thickness	Dependent on tissue type
Blade Speed	Zero to 200 strokes/min
Voltages	90/120 VAC, 60 Hz or 210/240 VAC, 50 Hz
Overall Dimensions	30 x 28 x 15 cm (11.8 x 11.0 x 5.9 in)
Weight	6.3 kg (13.9 lbs)

Order #	Product
W2 69-1010	McIlwain Mechanical Tissue Chopper, 115 V, 60 Hz
W2 69-1011	McIlwain Mechanical Tissue Chopper, 230 V, 50 Hz
Replacement Parts	
W2 69-1012	Cutting Blades, pkg. of 10
W2 69-1014	Cutting Table Disk (PVC, Darvik), pkg. of 10
W2 69-1015	Replacement Cutting Table
W2 69-1016	Cutting Table Clips
W2 69-1017	Spanner
W2 69-1013	Blade Holder

Warner Instruments Inc. • Phone (203) 776-0664 • Toll Free U.S. (800) 599-4203 • Fax (203) 776-1278 • **www.warneronline.com**

SZM 180

Stereo Zoom Microscope

W2 69-3101 Trinocular Zoom Stereo Microscope With Illumination Stand and Video Adapter

W2 69-3102 Trinocular Zoom Stereo Microscope With Boom Stand and Video Adapter

- High performance at an economical price
- Superior optical design with outstanding resolution and brilliantly sharp images
- Rugged all metal construction
- Excellent zoom range from 0.7x to 4.5x
- The parfocal zoom system keeps the image in constant focus while you zoom
- Zoom control knobs are conveniently side-mounted for smooth, comfortable operation
- Trinocular body with comfortable 45° inclination angle for fatigue-free viewing
- Trinocular body may be rotated 360° for group sessions
- Dual diopter adjustment of ±5 diopters enables you and your colleague to precisely set focus according to individual needs
- Interpupillary adjustment range from 55 to 75 mm
- Total magnification range extends from 3.5x to 90x
- Widefield eyepieces of 10x, 25x

Harvard Apparatus **SZM 180** Stereo Zoom Microscope provides outstanding quality at an affordable price. It features high-resolution optics and precise optical alignment that assures crisp sharp and flat 3-dimensional images.

Select from two different mounts. The standard mount has top halogen and bottom fluorescent illumination. The boom stand does not have any illumination, but permits working with large objects. You may also order the boom stand separately at a later date should you require it.

The Microscope is supplied complete with the following components: WF10X eyepiece; Trinocular zoom body, zoom range 0.7x – 4.5x; Video adapter with external C-mount, adjustable.

Specifications

Eyepieces	Widefield eyepieces of 10x and 25x
Objectives	Built-in zoom and attachable auxiliary lens
Zoom Range	From 0.7x to 4.5x
Illumination	Top halogen and bottom fluorescent, standard mount only
Video Capabilities	Built-in video and photographic port (lens and adapter required)
Shipping Dimension:	
W2 69-3101	490 x 390 x 275 mm (19 x 15 x 11 in)
W2 69-3102	Box #1 - 520 x 420 x 140 mm (20 x 16 x 5.5 in) Box #2 - 300 x 250 x195 mm (12 x 10 x 8 in)
Shipping Weight:	
W2 69-3101	9.5 kg (21 lbs)
W2 69-3102	Box #1 - 16.5 kg (36 lbs) Box #2 - 2.5 kg (6.5 lbs)

Order #	Product
W2 69-3101	SZM 180 Trinocular Zoom Stereo Microscope with Illumination Stand and Video Adapter
W2 69-3102	SZM 180 Trinocular Zoom Stereo Microscope with Boom Stand and Video Adapter
W2 69-3103	2x Auxiliary Lens for Zoom Stereo Microscopes
W2 69-3104	0.5x Auxiliary Lens for Zoom Stereo Microscopes
W2 69-3105	Adapter for Fiber Optics Ring Light or Fluorescent Ring Light
W2 69-3106	15W Halogen Lamp and Reflector
W2 69-3107	5W Fluorescent
W2 69-3108	Boom Stand for Stereo Microscope
W2 72-4666	Ringlight Adapter, 66 mm OD, for use with Ringlights, see pages 323 to 328
W2 69-3111	Microscope for Microforge

900 Series

Inverted Microscope

W2 69-3100 Inverted Microscope with Phase Contrast Objectives and Video/Photo Port

Ergonomically designed and precisely manufactured, yet simple to use, the Harvard Apparatus **SZM 180** Stereo Zoom Microscope provides versatility and high quality images for brightfield and phase/contrast observation. With standard built-in photographic and video port, the HAI 900 is the ideal instrument for tissue culture and other advanced applications.

Microscope is supplied complete with the following components: stand and observation head; WF10x eyepiece; 11x centering telescope; 4x Long working distance (LWD) plan objective and annulus; 10x LWD phase contrast plan objective and annulus; 25x LWD phase contrast plan objective and annulus; and 40x LWD phase contrast plan objective and annulus.

- Ideal for Tissue Culture and Cell Biology
- Long working distance Plan objectives (4x, 10x, 25x and 40x)
- Long working distance Plan phase objectives (10x, 25x and 40x)
- Optional SLR 35 mm photographic system
- Optional CCTV system
- Large mechanical stage with low position coaxial x-y movement
- Wide selection of filters
- Swing-out condenser to accommodate extra large objects

Specifications

Eyepieces	Paired WF10X eyepieces
Objectives	Choice of 10x, 25x and 40x, Plan brightfield long working distance objectives, Plan phase long working distance objective
Video Capabilities	Built-in video and photographic port (lens and adapter required)
Stage	Large graduated mechanical stage with low position x-y movement knob
Condenser	Centerable condenser with iris diaphragm and phase annulas ring slot, swing-out condenser holder with rack and pinion movement and safety stop
Filters	Filter disc with five positions
Diaphragm	Field Diaphragm and condensing lens
Illumination	Built-in 6V, 20W halogen illumination with intensity adjustment and lamp centering device
Shipping Dimensions	229 x 330 x 508 mm (9 x 13 x 20 in)
Shippinig Weight	16.5 kg (36 lbs)

Order #	Product
W2 69-3100	900 Series Inverted Microscope with Phase Contrast Objectives and Video/Photo Port
W2 64-0302	Stage Adapter for HAI 900 Microscope permits use of Series 20 Imaging and Recording Chambers
W2 69-3109	Replacement 6V/20 W Halogen Bulb for Inverted Microscope
W2 69-3110	Replacement Fuse 250V/1.5A for Inverted Microscope

Warner Instruments Inc. • Phone (203) 776-0664 • Toll Free U.S. (800) 599-4203 • Fax (203) 776-1278 • **www.warneronline.com**

Intralux® 5100

High Intensity Cold Halogen Light Source

- Compatible with all Volpi Fiber Optic Components
- Ergonomic design with small footprint
- Quick bulb replacement, reducing downtime
- Solid metal housing, designed for industrial use
- Certified for electronic and mechanical safety
- 150 watt cold light source with superior illumination intensity and long lamp life

Intralux® light sources have represented the best in Fiber Optic Cold Light Illumination the world for over 25 years. They provide reliable, dependable, high-intensity cold halogen light for use with all Volpi fiber optic components in microscopy applications.

The Intralux Series is equipped with the most advanced features and highest quality components available. It includes InfraRed Reflecting Filters to ensure the coldest light possible and the unique patented Crescent Shaped Diaphragm, which provides constant color temperature and light emitting angle, and continuous intensity adjustment.

Fiber optic components consist of:

- **Ringlights**
- **Goosnecks (sliding Sleeve: Volpi Patent)**
- **Flexible Light Guides**
- **Backlights**

Specifications

Average lamp life (calculated value, in continuous operation at line voltage 230V / 121V / 100V):	
110% intensity	100 hours
100% intensity	200 hours
90% intensity	520 hours
80% intensity	1700 hours
75% intensity	3600 hours
Color temperature at 110% intensity	3433K
Illumination intensity at 110% voltage at lightguide input (DIN 58141-10)	12.3 M Lux
Maximum illuminated light guide-Ø	13 mm
Mechanical light guide connector Ø	15 mm
Light adjustment	electrical, 8-step switch 75 to 110% Crescent shaped diaphragm (Volpi Patent) 16-steps
Halogen Reflector Lamp	EKE 21 V/150 W
Line Voltages ±10%	230 V, 50 Hz or 121 V, 60 Hz or 100 V, 60 Hz
Power Consumption	190 W
Protection Class	1
Weight	4.6 kg (10 lbs)
Housing	Metal, powder coated, color RAL 9002
Approvals	UL61010-1, CAN/CSA 61010-1,CE/Product Safety : IEC/EN 61010-1:2001 EMC: Emission: IEC/CISPR 11, Class B/Immunity: IEC 61000-4-2 to 6 and 11

Order #	Product
W2 72-6195	Intralux® 5100 Light Source, USA, 121 V, 60Hz
W2 72-6196	Intralux® 5100 Light Source, EURO, 230V, 50Hz
W2 72-6198	Intralux® 5100 Light Source, CH, 230V, 50Hz
W2 72-6197	Intralux® 5100 Light Source, JAP, 100V, 60Hz
W2 72-0227	Halogen Spare Lamp EKE 21V/150W

V-Lux 1000 and IWL-500e

Fiber Optic Cold Light Sources

V-Lux 1000

Intralux IWL-500e

- For Microscope Illumination
- Constant color temperature and light emitting angle
- Continuous intensity adjustment
- Low-cost alternative to the Intralux series
- Use with fiber optic ringlights, goosenecks, and flexible light guides

V-Lux 1000 Cold Light Source

The **V-Lux 1000** is a low-cost quality fiber optic cold light source featuring many high-end features such as compact design, constant color temperature, long lamp life and low noise/vibration. It is ideal for any microscopy applications. The V-Lux 1000 will provide reliable, dependable, high-intensity cold halogen light for use with all Volpi fiber optic components in microscopy applications. Although it is factory equipped with DDL Lamps, EKE bulbs may be easily substituted for slightly more light output. Has integrated resettable fuse transformer.

Specifications

Uniformly Illuminated Light Guide Diameter	13 mm
Rated Lamp Life	DDL 800 hrs*, EKE 350 hrs*
Color Temperature	DDL 3120°K, EKE 3190°K, constant
Light Adjustment	Crescent shaped diaphragm
Lamp	DDL-20V/150W or EKE-21V/150W
Dimensions, H x W x D	9.5 x 17.1 x 21.0 cm (3.75 x 6.75 x 8.25 in)
Weight	4.5 kg (9.92 lb)

** Average of continuous operation*

Order #	Product
W2 72-0215	V-Lux 1000, 120 V, USA/Canada
W2 72-0216	V-Lux 1000, 230 V*
W2 72-0217	V-Lux 1000, 230 V**
W2 72-0218	V-Lux 1000, 230 V***
W2 72-0231	V-Lux 1000, 230 V****
W2 72-0232	V-Lux 1000, 230 V*****

Power cord is hard-wired to light source.

* *Argentina/Austria/Belgium/Brazil/China/Denmark/Finland/France/Germany/Indonesia/Netherlands/Norway/Sweden/Switzerland/Thailand/Vietnam*
** *Australia/New Zealand/Fiji*
*** *UK*
**** *South Africa*
***** *Ireland/Italy*

- High intensity
- Cold, metal halide light source
- Long lamp life
- Stable light output

Intralux IWL-500e White Light Source

The **Intralux IWL-500e** is a low-cost 50 watt metal halide light source which boasts over 5500°K temperature and 3500-hr lamp life. This metal halide light source features a compact design and produces three times the intensity of 150 watt Halogen sources. Excellent choice for use with the Fiber Optic Bifurcated Gooseneck.

Note: All Volpi Light Sources are compatible with all Volpi Fiber Optic Components.

Specifications

Rated Lamp Life	3500 hrs
Color Temperature	5500°K (±900°K)
Light Adjustment	Continuous intensity crescent shaped diaphragm
Lamp	120 V/50 W or 230 V/50 W
Dimensions, H x W x D	12.2 x 22.1 x 22.4 cm (4.8 x 8.7 x 8.8 in)
Weight	3.31 kg (7.3 lb)

Order #	Product
W2 72-0234	Intralux IWL-500e, 120 V, USA/Canada
W2 72-0235	Intralux IWL-500e, 230 V, Europe
W2 72-6194	Replacement Lamp for Intralux IWL-500e

Warner Instruments Inc. • Phone (203) 776-0664 • Toll Free U.S. (800) 599-4203 • Fax (203) 776-1278 • **www.warneronline.com**

Intralux DC 1100 and Filters

Fiber Optic Cold Light Sources

- Voltage regulated fiber optic cold light source with remote control of light intensity adjustment
- Use with fiber optic ringlights, goosenecks, flexible light guides, and backlights.
- Equipped with EKE bulb
- °Kelvin temp dependent on voltage setting
- Digital RS 232 interface with 1023-step adjustment
- Low noise/vibration
- Compact ergonomic design/metal housing

Intralux DC 1100 Light Source

The **Intralux DC 1100** is a high-end voltage regulated light source with digital RS 232 interface and 1023-step light intensity adjustment. Can be used in a variety of applications requiring stable light output, manually or remotely. DC Regulation ensures stable light output. Patented Crescent Shaped Diaphragm allows continuous intensity adjustment and constant color temperature.

Order #	Product
W2 72-0236	Intralux DC 1100 Light Source , 120 V USA/Canada
W2 72-0237	Intralux DC 1100, 230 V Euro*

** Note: Power cord not included; specific country power cords available on page 322.*

- **Blue Filters** enhance red and yellow objects and lighten blue and green objects
- **Red Filters** will darken blue and green objects and are useful for black and white applications
- **Green Filters** increase contrast for blue and red objects and brighten yellow and green objects
- **Yellow Filters** of specific band widths may be used as a safe light when working with photosensitive materials
- **Daylight Conversion Filters** increase the Kelvin Temperature of the halogen light to 5500°K, which is daylight. Daylight Filters reduce glare from highly reflective material such as muscle tissue and metals

Light Source Filters

Light Source Filters provide contrast enhancement. When the composition of an object is made of two or more colors, a filter may be used to darken the color that is most important and, therefore, be able to observe it better. When the composition of an object is pale, a filter of the opposite or complementary color may enhance the detail. Specifically, when the composition of the object is highly dense and color saturated, a filter of the same color will most likely enhance the detail on the object. Custom filters of a specific band width are also available upon request.

Order #	Product
W2 72-0219	Blank Filter Holder for Intralux 5100/DC 1100
W2 72-0220	Blue Filter for Intralux 5100/DC 1100
W2 72-0221	Red Filter for Intralux 5100/DC 1100
W2 72-0222	Green Filter for Intralux 5100/DC 1100
W2 72-0223	Yellow Filter for Intralux 5100/DC 1100
W2 72-0224	Daylight Filter for Intralux 5100/DC 1100

Light Source Spare Parts and Accessories

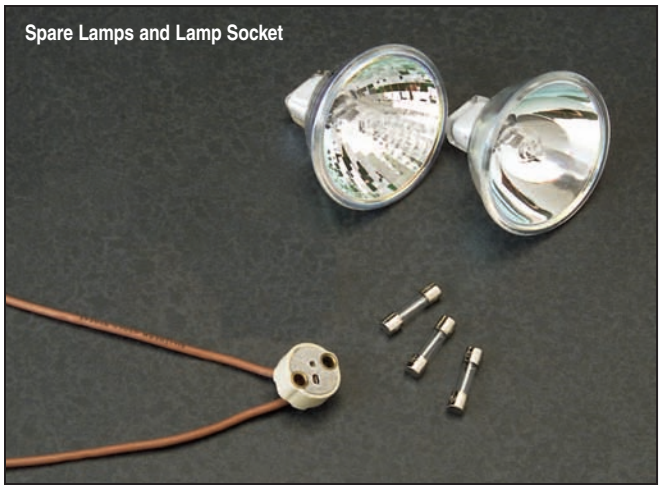
Spare Lamps and Lamp Socket

Ring Light Adapters

Spare Lamps and Power Cords

Order #	Product
W2 72-0227	EKE Spare Lamp for Intralux 5100 /V-Lux 1000/Intralux DC 1100 (21 V/150 W)
W2 72-0226	DDL Spare Lamp for Intralux 5100 /V-Lux 1000 (20 V/150 W)
W2 72-0356	Spare Lamp Socket-Round for Intralux 5100 /V-Lux 1000/Intralux DC 1100
W2 72-0348	Power Cord, United Kingdom
W2 72-0349	Power Cord, France
W2 72-0350	Power Cord, Italy
W2 72-0351	Power Cord, Switzerland
W2 72-0352	Power Cord, Germany
W2 72-0353	Power Cord, The Netherlands
W2 72-0354	Power Cord, Spain/Portugal

- Ringlight adapters available for all brand microscopes
- Provide direct and indirect mounting
- Low-Cost

Ringlight Adapters

Used with Standard/Compact and 4-Point Standard Ringlights for attachment to all brand microscopes. If your microscope is not listed here, please contact customer service for assistance.

Order #	Product
W2 72-4666	Ringlight Adapter for SZM 180 Stereo Zoom Microscopes, see page 317
W2 72-0249	Ringlight Adapter for Leica Classic Stereo Zoom 1-5 without Attachment Lens
W2 72-0250	Ringlight Adapter for Leica New Family SZ4/SZ6/Photo/Plus without Attachment Lens
W2 72-0305	Ringlight Adapter for Leica New Family SZ4/SZ6/Photo/Plus with Attachment Lens
W2 72-0251	Ringlight Adapter for Leica Stereo Zoom 7/GZ7 without Attachment Lens
W2 72-0252	Ringlight Adapter for Leica M3B/C/Z; Leica MZ6 Achromatic 0.32x/0.5x/0.63x/0.8x/1.0x
W2 72-0257	Ringlight Adapter for Olympus SZ/ without Attachment Lens
W2 72-0258	Ringlight Adapter for Olympus SZH9/SZH12 and Nikon SMZ Series without Attachment Lens

Note: *All Volpi Light Sources are compatible with all Volpi Fiber Optic Components.*

Fiber Optic Ringlights

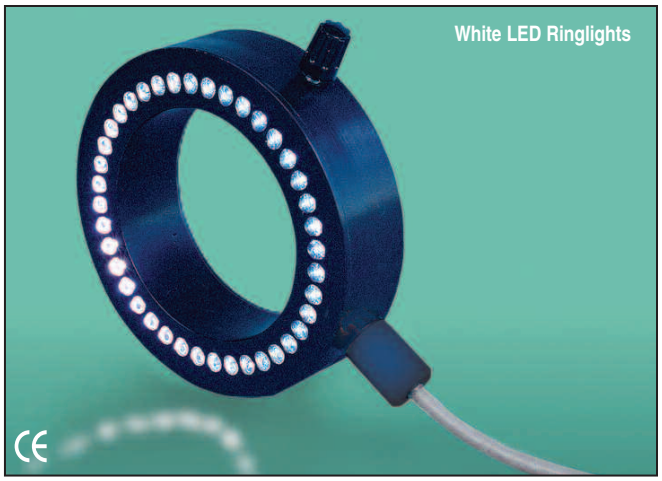

- 25 to 90 mm working distance
- Uniform and shadow-free illumination
- Full-circular
- Adaptable to all microscope brands

Standard Ringlight

Full circular glass fiber ringlight provides homogeneous, shadow-free illumination for working distances of 25 to 90 mm. Inside diameter is 66 mm for mounting on all microscopes through a series of ringlight adapters listed on facing page.

Order #	Product
W2 72-0238	Standard Ringlight with 750 mm (30 in) flexible length
W2 72-0239	Standard Ringlight with 1200 mm (48 in) flexible length
W2 72-0240	Standard Ringlight with 2400 mm (96 in) flexible length

- Compact, Metal Design
- Flicker-Free Light
- 7,000 to 10,000 LED life
- 7800˚K Temp
- Working Distance Range of 30 to 150 mm
- Adaptable to all microscopes

White LED Ringlights

White Light Emitting Diodes (LEDs) are now available in a ringlight to produce uniform, shadow-free illumination comparable to that of fiber optic ringlights. This exciting new technology is available in 5500˚K Temperature (Daylight) and 7800˚K Temperature for working distances of 30-150 mm. Metal housing design produces minimal heat for cool light illumination. Powered with an 8W/24V DC power supply (included), these ringlights offer flicker-free illumination. The most unique feature of these White LEDs is by far their rated life of 7,000-10,000 hours. White LED ringlights have the standard 66 mm inside diameter and are adaptable to all microscopes and lenses through a series of available ringlight adapters.

Order #	Product
W2 72-4656	Standard White LED Ringlight, 30-70 mm Working Distance
W2 72-4657	Diffuse Standard White LED Ringlight, 30-90 mm Working Distance
W2 72-4658	Spot/Focused White LED Ringlight, 70-160 mm Working Distance
W2 72-4659	Daylight LED Ringlight-5500°K Temp - Short Working Distance, 30-70 mm Working Distance
W2 72-4660	Daylight LED Ringlight-5500°K Temp - Long Working Distance, 70-160 mm Working Distance
W2 72-4661	Rheostat Accessory for use with all LED Ringlights
W2 72-4662	Ring Polarizer Set with Glass Analyzer for all LED Ringlights

Fiber Optic Ringlights (continued)

- Compact design
- 15 to 70 mm working distances
- Uniform and shadow-free illumination
- Adaptable to all microscope brands

Compact Ringlight

Full circular glass fiber ringlight provides homogenous, shadow-free illumination for working distances of 15 to 70 mm. Inside diameter is 66 mm for mounting on all microscopes through a series of ringlight adapters listed on page 322. Standard Flexible length is 750 mm (30 in). Longer lengths available.

Order #	Product
W2 72-0233	M10 Compact Ringlight

- Depth perception
- 70 to 100 mm working distance
- Adaptable to all microscope brands

4-Point Standard Ringlight

Standard ringlight with four fiber points provides illumination with depth perception for working distances of 70 to 100 mm. Inside diameter is 66 mm for mounting on all microscopes through a series of ringlight adapters listed on page 322. Standard Flexible length is 750 mm (30 in). Longer lengths available.

Order #	Product
W2 72-0248	4-Point Standard Ringlight

Fiber Optic Ringlights (continued)

- Small diameter
- Full circular
- 5 to 175 mm working distances
- Shadow-free
- Direct mounting for 20 to 32 mm objectives

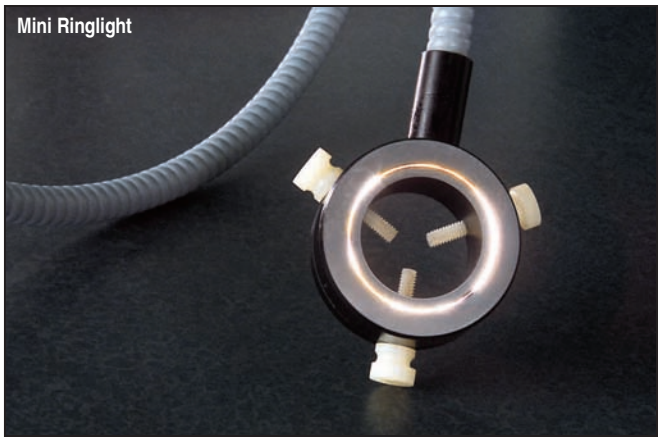

Mini Ringlight

Small full circular glass fiber ringlight provides homogeneous, shadow-free illumination for working distances of 5 to 25 mm. Long Working Distance version is available for distances of 25 to 175 mm. Can be used for fiber optic illumination on Compound Microscope objectives. Mounting diameter ranges from 20 to 32 mm with the presence of 3 mounting screws without the need for adapters. Standard Flexible length is 900 mm (40 in). Longer lengths available.

Order #	Product
W2 72-0246	Short Working Distance Mini Ringlight
W2 72-0247	Long Working Distance Mini Ringlight

- Large diameter
- Full circular
- 50 to 120 mm working distance
- Diffuse light
- High intensity

SMD/MAXI Ringlight

Large full circular diameter glass fiber ringlight that provides homogenous, shadow-free illumination for working distances of 50 to 120 mm. Large diameter and shallow fiber angle produces wonderful darkfield effect on large surface areas. Inside diameter is 150 mm and can be adapted to SMD stations and stereomicroscope columns. Standard Flexible length is 480 mm (19 in) with longer lengths available on request.

Order #	Product
W2 72-0245	SMD/MAXI Ringlight

Ringlights and Accessories

- Ergonomic
- Long working distance starting at 100 mm
- Direct mounting to Olympus

Ergo/Olympus SZ/SD Ringlight

Tapered ringlight for direct mounting on Olympus SZ/SD Microscopes with minimum loss of working distance. Flexible length exits at 45° angle allowing maximum work space. Long Working distance starting at 100 mm with long flexible lengths available. Adapter included.

Order #	Product
W2 72-0242	Ergo/Olympus SZ/SD Ringlight

Ergo/Olympus SZ/SD Ringlight

- Reduces or eliminates unwanted reflections
- Extends standard ringlight working distance range
- Used with standard, compact and 4-point standard ringlights

Accessories for Standard/Compact and 4-Point Ringlights

Ring Polarizer Set

Eliminates unwanted reflections of highly reflecting materials such as tissue and metallic objects. Glass analyzer is used with plastic polarizer for the best possible cross-polarization effect. Can be used with Standard, Compact, and 4-Point Standard Ringlights.

Toric Lens

Extends the working distance of Standard and Compact Ringlights from 90 to 150 mm. Longer distance ringlights are also available as an alternative.

Diffuser

Reduces unwanted reflections of highly reflecting materials such as tissue and metallic objects. Can be used with Standard, Compact, and 4-Point Standard Ringlights.

Order #	Product
W2 72-0262	Ring Polarizer Set for Standard/Compact Ringlights
W2 72-0265	Toric Lens for Standard/Compact Ringlights
W2 72-0264	Diffuser for Standard/Compact Ringlights

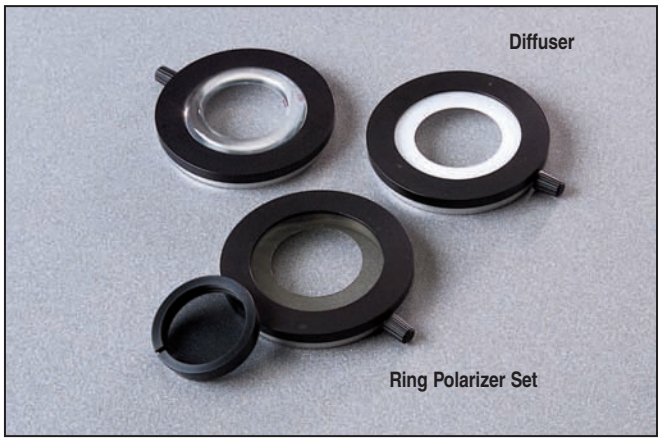

Note: *All Volpi Light Sources are compatible with all Volpi Fiber Optic Components.*

Gooseneck Light Guides

Gooseneck Light Guides

Gooseneck light guides provide fiber optic incident illumination using semi-obedient, self-supporting arms with no spring-back action. You can position each arm independently and with the key system in place, there is no rotation. Single Arm and bifurcated Goosenecks are available with 4.7 mm and 5.4 mm diameter.

Special Volpi Patent: Sliding Sleeve allows fiber bundles to move independently of the outer tubing for minimal fiber breakage over time. Gooseneck Arms are repairable. Light sources are sold separately.

Order #	Product
W2 72-0268	Single Arm Gooseneck Light Guide, Black, 4.7 mm fiber diameter
W2 72-0266	Bifurcated Gooseneck Light Guide, Gray, 5.4 mm fiber diameter (each arm)
W2 72-0267	Bifurcated Gooseneck Light Guide, Black, 4.7 mm fiber diameter (each arm)

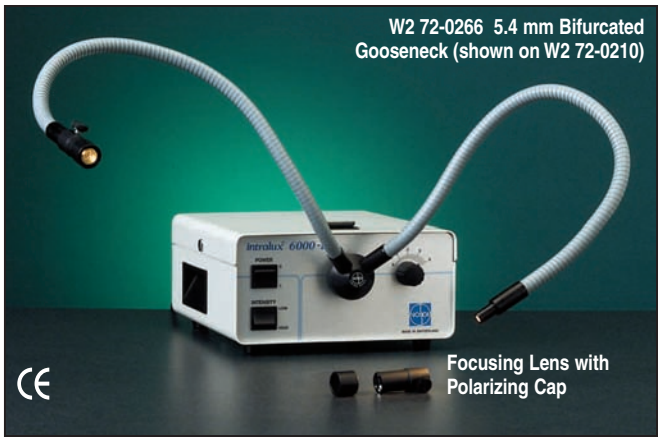

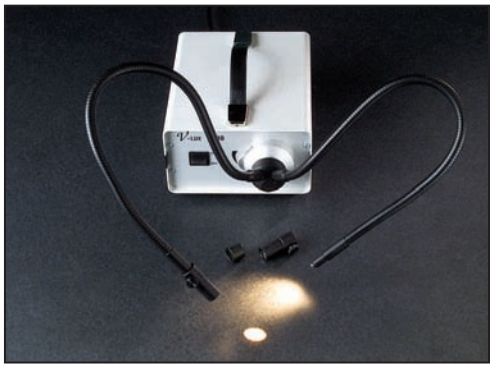

Gooseneck Accessories

Standard Focusing Lens: A spherical lens used to focus light to a concentrated spot.

Polarizing Cap: Fits onto focusing lens.

Order #	Product
W2 72-0269	Standard Focusing Lens
W2 72-0304	Polarizing Cap for Standard Focusing Lens For Modular Accessory System, see page 329

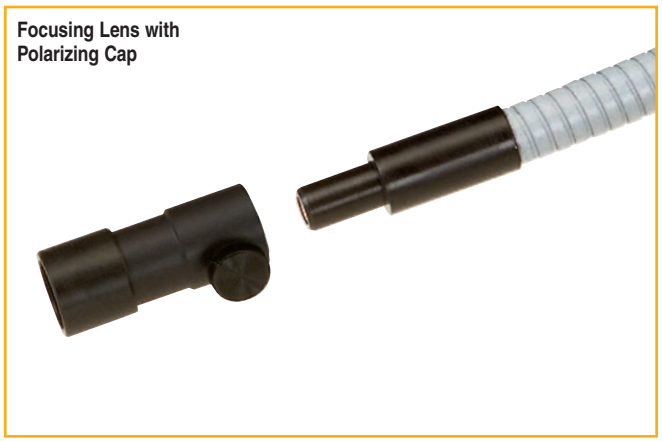

Gooseneck Light Guides (continued)

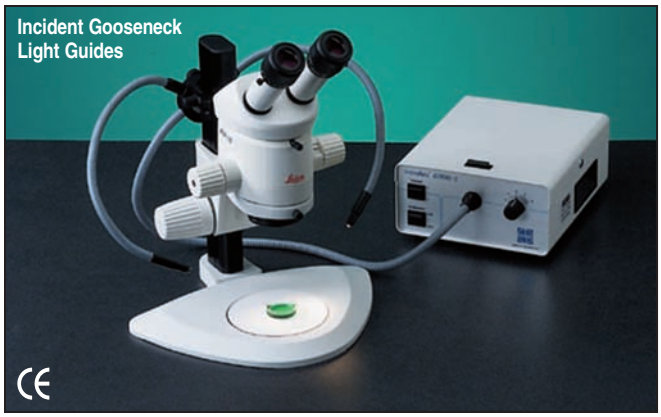

- Bifurcated Gooseneck and flexible light guide combination
- Attachable to columns of all brand microscopes through available adapters
- Great flexibility in the placement of light source
- Available in different lengths
- Uses standard Gooseneck accessories

Incident Gooseneck Light Guides

This combination of a Semi-Obedient Bifurcated Gooseneck and a Flexible Light Guide provides incident illumination. Fiber Optic **Incident Goosenecks** attach to the columns of microscopes or other work station columns with specialized adapters. Each arm can be positioned and adjusted independently. The flexible length size can vary to allow the placement of the light source away from the microscope and work station.

Utilizes standard Gooseneck accessories such as Focusing Lens W2 72-0269, Polarizing Caps W2 72-0304 and Modular Accessory System found on pages 327 and 329. Light sources are sold separately.

Order #	Product
W2 72-0329	Incident Gooseneck Light Guide, Gray, 4.7 mm fiber diameter (each arm), 75 cm (30 in)
W2 72-0330	Incident Gooseneck Light Guide, Gray, 4.7 mm fiber diameter (each arm), 100 cm (40 in)
W2 72-0331	Incident Gooseneck Light Guide, Gray, 4.7 mm fiber diameter (each arm), 150 cm (60 in)
W2 72-0332	Incident Gooseneck Light Guide, Gray, 4.7 mm fiber diameter (each arm), 200 cm (80 in)
W2 72-0333	Incident Gooseneck Light Guide Adapter for 20 to 25 mm Round Columns
W2 72-0334	Incident Gooseneck Light Guide Adapter for 32 mm Round Columns
W2 72-0335	Incident Gooseneck Light Guide Adapter for Nikon SM5/6 and SMZ 6/10
W2 72-0336	Incident Gooseneck Light Guide Adapter for Olympus SZX9/12
W2 72-0308	Incident Gooseneck Articulated Arm Support Adapter for Leica G26, MS5, M26, M28, M212

- Point illumination
- Highly flexible
- PVC metal tubing provides durability.
- 3 to 13 mm fiber diameters
- Standard and custom lengths available

Flexible Light Guides

Highly flexible and durable light guides available in 3 to 13 mm of fiber diameters and various standard and custom lengths. Outer tubing is composed of PVC metal tubing to provide both flexibility and protection. Standard single arm and twin arm versions available. Customized versions are available upon request.

Flexible Light Guides

Fiber Diameter (mm)	**3**	**5**	**8**	**10**	**13**
Bushing Diameter	**5**	**10**	**10**	**13**	**16**
Single Arm Lengths					
50 cm (20 in)	**W2 72-0283**	**W2 72-0287**	**W2 72-0291**	**W2 72-0295**	**W2 72-0299**
100 cm (40 in)	**W2 72-0284**	**W2 72-0288**	**W2 72-0292**	**W2 72-0296**	**W2 72-0300**
150 cm (60 in)	**W2 72-0285**	**W2 72-0289**	**W2 72-0293**	**W2 72-0297**	**W2 72-0301**
200 cm (80 in)	**W2 72-0286**	**W2 72-0290**	**W2 72-0294**	**W2 72-0298**	**W2 72-0302**
Twin Arm Lengths					
100 cm (40 in)	–	**W2 72-0313**	**W2 72-0316**	–	–
150 cm (60 in)	–	**W2 72-0314**	**W2 72-0317**	–	–
200 cm (80 in)	–	**W2 72-0315**	**W2 72-0318**	–	–

Light Guide Accessories

- Fixed point illumination
- Accurate adjustment for quick, simple and precise positioning
- Unrestricted movement – 220 mm radius of action
- Very durable

Articulating Arm with Heavy Steel Base

Articulating Support Arm provides unrestricted movement and accurate fine adjustment for fixed point illumination. Adjustment is simple and precise with 220 mm radius of action. Articulating Arms are available with M6/M6 and M6/M8 thread ends. Flexible Light Guides can be attached with small (9 to 12 mm OD) and large (11 to 16 mm OD) holders depending on flexible light guide outer ferrule diameters.

Order #	Product
W2 72-0323	Articulated Support Arm, M6/M6 Thread
W2 72-0328	Articulated Support Arm, M6/M8 Thread
W2 72-0324	Heavy Steel Base for Articulated Support Arm
W2 72-0325	Holder for Articulated Support Arm, ferrule diameter 9 to 12 mm (0.35 to 0.47 in)
W2 72-0326	Holder for Articulated Support Arm, ferrule diameter 11 to 16 mm (0.43 to 0.63 in)

Modular Accessory System

- Use with Goosenecks and up to 8 mm OD Flexible Light Guides
- Allows combination of filters and other accessories
- Very versatile

Modular Accessory System

Modular Holder has a 10 mm mounting diameter and attaches onto ends of goosenecks and up to 8 mm OD flexible light guides. Modular Accessory Holder and each of the Modular Accessories are threaded to accept one another. Modular accessories include the Modular color filters, Modular focusing lens, Modular diffuser, Modular polarizing filter, and Modular iris diaphragm. One or all can be attached at any one time. Custom filters are also available upon request.

Order #	Product
W2 72-0270	Modular Accessory Holder
W2 72-0271	Modular Focusing Lens
W2 72-0272	Modular Iris Diaphragm
W2 72-0273	Modular Polarizing Filter
W2 72-0274	Modular Daylight Filter
W2 72-0275	Modular Blue Filter
W2 72-0276	Modular Red Filter
W2 72-0277	Modular Green Filter
W2 72-0278	Modular Yellow Filter
W2 72-0280	Modular Blank Filter
W2 72-0279	Modular Diffuser

Note: *All Volpi Light Sources are compatible with all Volpi Fiber Optic Components.*

Backlights and Base

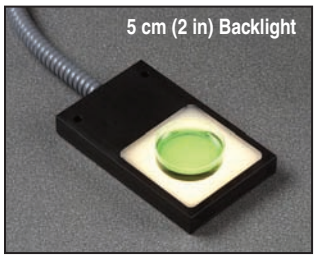

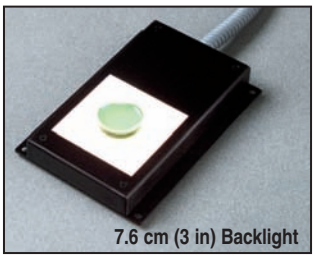

- Homogeneous, diffuse backlight illumination
- Used in the image processing, brightfield illumination on stereo microscopes, pattern recognition of different transparencies, area recognition of different colors, side illumination, dimensional gauging, shape verification, etc.

Glass Light Fiber Backlights

Glass Fiber Backlights provide homogeneous, diffuse illumination. Glass fiber used is extremely durable and heat tolerant. Can be adapted to most brand microscope bases.

Available in three sizes: 5 x 5 cm (2 x 2 in), 7.6 x 7.6 cm (3 x 3 in), and 12.7 x 12.7 cm (5 x 5 in). Additional specifications listed below.

Specifications

	W2 72-0342	W2 72-0343	W2 72-0344
Product	2 inch Backlight	3 inch Backlight	5 inch Backlight
Homogeneous Illumination Field	5 x 5 cm (2 x 2 in)	7.6 x 7.6 cm (3 x 3 in)	12.7 x 12.7 cm (5 x 5 in)
Dimensions, H x W x D	1.3 x 10.2 x 6.4 cm (0.5 x 4.0 x 2.5 in)	2.3 x 17.2 x 12.1 cm (0.9 x 6.75 x 4.75 in)	2.3 x 22.2 x 17.2 cm (0.9 x 8.75 x 6.75 in)
Uniformity	±10%	±10%	±10%
Fixing Holes (4 each) Diameter	6.3 mm (0.25 in)	6.3 mm (0.25 in)	6.3 mm (0.25 in)
Flexible Light Guide (Met/PVC)	91.4 cm (36 in)	91.4 cm (36 in)	91.4 cm (36 in)
Light Source Adapter	Intralux Series	Intralux Series	Intralux Series

Order #	Product
W2 72-0342	Glass Fiber Backlight, 5 x 5 cm (2 x 2 in)
W2 72-0343	Glass Fiber Backlight, 7.6 x 7.6 cm (3 x 3 in)
W2 72-0344	Glass Fiber Backlight, 12.7 x 12.7 cm (5 x 5 in)

- Transmitted bright/darkfield illumination
- Uses standard/compact ringlight illumination
- Low cost alternative
- Compact design
- Adapts to all brand name microscopes

Brightfield/Darkfield Base

This is a low-cost, intense, contrast-rich, transmitted, light **Bright/Darkfield Base** used with Standard or Compact Fiber Optic Ringlights. It provides transmitted bright/darkfield illumination. Easily accessible knob allows quick and easy change between brightfield and darkfield. Adapts to all brand name microscopes.

Order #	Product
W2 72-0337	Bright/Darkfield Base
W2 72-0339	Polarizer to Base
W2 72-0340	Diaphragm to Objective, 0.5/0.63X
W2 72-0341	Diaphragm to Objective, 1.5/2.0X

Note: *All Volpi Light Sources are compatible with all Volpi Fiber Optic Components.*

Warner Model Number Index

Warner Model	Order #	Page No.
111	W2 64-0275	70
111-KIT	W2 64-0378	46, 47, 70
1302	W2 69-3006	280
1U9924M-12	W2 64-0598	191
2100	W2 64-0042	159
2510	W2 64-0043	157
2U9330	W2 64-0559	189
3110	W2 64-1423	161
3SG700-10	W2 64-0120	81
3SG700-5	W2 64-0119	81
3SHD-22F/15	W2 64-1411	66
5101-01G	W2 64-0015	135
5101-100M	W2 64-0016	135
5101-10G	W2 64-0014	135
5101-10GB	W2 64-0017	135
7250V	W2 64-0031	153
7251I	W2 64-0032	153
7255DI	W2 64-0030	153
7259C	W2 64-0033	153
725MC	W2 64-0029	153
782	W2 69-3001	278
928	W2 69-3000	278
ABR-1	W2 64-1426	69
ACC-1	W2 64-1427	96
AG10W	W2 64-1319	295
AG15W	W2 64-1320	295
AG8W	W2 64-1318	295
AGT10W	W2 64-1321	295
AK15	W2 69-0448	225
AO16 1.0	W2 69-0867	303
AO16 1.2	W2 69-0868	303
AO16 1.2	W2 69-0869	303
AR-1	W2 64-0350	114, 126
AR-2	W2 64-1455	126
AR-4	W2 64-0351	115, 116, 124
AR-4	W2 64-0351	126
BAC-1	W2 64-1606	98, 109
BA-D15X10	W2 64-0615	53
BA-R15	W2 64-0612	53
BA-R3	W2 64-0611	53
BA-S2.5X10	W2 64-0614	53
BA-S3X7	W2 64-0613	53
BB-15	W2 64-0040	159
BC-535	W2 64-0432	139
BCH-13A	W2 64-0400	137, 141
BCH-22A	W2 64-0401	137
BCH-22A	W2 64-0401	141
BCH-M13	W2 64-0451	137
BCH-M13	W2 64-0451	147
BCH-M22	W2 64-0453	137
BCH-M22	W2 64-0453	147
BCH-P	W2 64-0423	137, 142
BLM-ST	W2 64-0067	146
BLM-TC	W2 64-0450	137
BLM-TC	W2 64-0450	147
BPM-1	W2 64-1586	12, 13, 156
BPS-2	W2 64-0431	143
BSC-ACC-KIT	W2 65-0088	127, 129
BSC-AIR	W2 65-0078	129
BSC-BU	W2 65-0073	127, 129
BSC-BUW	W2 65-1525	129
BSC-CABLE	W2 65-0091	129
BSC-G10	W2 65-0082	129
BSC-HE	W2 65-0080	129
BSC-HT	W2 65-0075	128, 129
BSC-HT-AG	W2 65-0084	129
BSC-HTC	W2 65-0083	129
BSC-MESH	W2 65-0090	129
BSC-ORING	W2 65-0079	129
BSC-PC	W2 65-0076	127, 129
BSC-PC-VAL	W2 65-0087	129
BSC-T2	W2 65-0098	97, 123, 129
BSC-T2A	W2 65-0016	97, 123
BSC-T3	W2 65-0057	97, 123, 129
BSC-T3A	W2 65-0056	97, 123
BSC-TH	W2 65-0055	123
BSC-TUBE	W2 65-0081	129
BSC-ZT	W2 65-0074	128, 129
BSC-ZTC	W2 65-0086	129
CB-10	W2 64-0312	15
CB-10/2	W2 64-0313	15
CB-1N	W2 64-0311	15
CB-20	W2 64-0315	15
CB-20/2	W2 64-0316	15
CB-2LZ	W2 64-0317	15
CB-2N	W2 64-0314	15
CC-102	W2 64-1425	47, 51, 110, 210
CC-15	W2 64-0303	58, 110
CC-28	W2 64-0106	58, 95, 110, 114-116, 119, 124, 125
CC-35	W2 64-0109	58, 95, 110
CD13A-150	W2 64-0410	137
CD13A-200	W2 64-0409	137
CD13A-250	W2 64-0408	137
CD22A-150	W2 64-0413	137
CD22A-200	W2 64-0412	137
CD22A-250	W2 64-0411	137
CD-P150	W2 64-0427	142
CD-P-150	W2 64-0427	137
CD-P200	W2 64-0428	142
CD-P-200	W2 64-0428	137
CD-P250	W2 64-0429	142
CD-P-250	W2 64-0429	137
CF13A-150	W2 64-0416	137
CF13A-200	W2 64-0415	137
CF13A-250	W2 64-0414	137
CF22A-150	W2 64-0419	137
CF22A-200	W2 64-0418	137
CF22A-250	W2 64-0417	137
CFL-6	W2 64-0166	79, 86
CIS-10-F	W2 69-0112	99
CL-100	W2 64-0352	96, 101, 103
CM-1	W2 64-0024	137
CM-1/10	W2 64-0024	148
CM-1/100	W2 64-0025	148
CM-3	W2 64-0026	137
CM-3/10	W2 64-0026	148
CM-3/100	W2 64-0027	148
CP13A-150	W2 64-0404	137
CP13A-200	W2 64-0403	137
CP13A-250	W2 64-0402	137
CP22A-150	W2 64-0407	137
CP22A-200	W2 64-0406	137
CP22A-250	W2 64-0405	137
CP-P150	W2 64-0424	142
CP-P-150	W2 64-0424	137
CP-P200	W2 64-0425	142
CP-P-200	W2 64-0425	137
CP-P250	W2 64-0426	142
CP-P-250	W2 64-0426	137
CPS-27	W2 64-1451	34
CPS-27L	W2 64-1450	36
CPS-27N	W2 64-1452	37
CR-15	W2 64-0276	19, 58
CS-12R	W2 64-0702	28, 49, 65
CS-12R15	W2 64-0712	49, 65
CS-15R	W2 64-0703	19, 28, 46, 49, 65
CS-15R15	W2 64-0713	49, 65
CS-18R	W2 64-0384	46, 49, 50, 65
CS-18R15	W2 64-0714	49, 50, 65
CS-22/30	W2 64-0706	43, 65
CS-22/3015	W2 64-0716	65
CS-22/40	W2 64-0707	25-27, 29, 31, 32, 43, 53, 65
CS-22/4015	W2 64-0717	65
CS-22/50	W2 64-0708	18, 33, 65
CS-22S	W2 64-0704	20, 26, 65
CS-24/50	W2 64-0709	34, 36-38, 39, 40, 65
CS-24/60	W2 64-0710	35, 65
CS-25R	W2 64-0705	20-23, 49-51, 53, 65, 123
CS-25R15	W2 64-0715	49-51, 65
CS-30R	W2 64-1499	43, 65
CS-40R	W2 64-1500	43, 65, 126
CS-5R	W2 64-0700	65

Warner Model Number Index

Warner Model	Order #	Page No.
CS-8R	W2 64-0701	65
CS-GLASS-2	W2 64-0069	123
CSH-1	W2 64-1592	119
CSMI	W2 65-0101	120
D121-11	W2 65-0337	211
D3512B	W2 64-0761	126
D3512P	W2 64-0757	126
D3522B	W2 64-0762	46, 47, 126
D3522P	W2 64-0758	46, 47, 126
D5030B	W2 64-0763	126
D5030P	W2 64-0759	126
D5040B	W2 64-0764	126
D5040P	W2 64-0760	54, 125, 126
DC-6	W2 64-0142	79
DH-35	W2 64-0110	46, 47, 114
DH-35i	W2 64-0349	46, 47, 115
DH-40i	W2 64-0388	46, 47, 116
DM MC6	W2 69-0950	209
DM MC6 HV	W2 69-0939	203
DM MC6 HV	W2 69-0943	203
DM MC6 HV	W2 69-0947	203
DM MC6 LV	W2 69-0938	203
DM MC6 LV	W2 69-0942	203
DM MC6 LV	W2 69-0946	203
DM6	W2 69-0952	209
DM660	W2 69-0932	209
DN/10	W2 64-0158	84
DN/20M	W2 64-0159	84
DN/30M	W2 64-0160	84
DN/5	W2 64-0157	84
DN/60M	W2 64-0161	84
D-ORING-1	W2 65-0066	123
D-ORING-2	W2 65-0067	123
DP-301	W2 64-0044	160
DP-304	W2 64-0045	160
DP-311	W2 64-1422	161
DS2A	W2 65-0329	211
DS3	W2 65-0550	211
E200	W2 64-1304	293
E201	W2 64-1305	293
E202	W2 64-1306	293
E203	W2 64-1307	293
E204	W2 64-1308	293
E205	W2 64-1309	293
E206	W2 64-1310	293
E207	W2 64-1311	294
E208	W2 64-1312	294
E210	W2 64-1313	293
E242	W2 64-1314	294
E243	W2 64-1315	294
E244	W2 64-1316	294
E255	W2 64-1317	293
E45W-F10VH	W2 64-1051	153
E45W-F12VH	W2 64-1052	153
E45W-F20VH	W2 64-1054	153
EC-800	W2 64-0035	201
EC-800LV	W2 64-0036	201
EC-825A	W2 64-1605	201
EH 100	W2 69-3024	283
EM-CSYS	W2 69-0955	205
EM-LVSYS	W2 69-0968	205
EOS	W2 64-1463	258
EP MC6	W2 69-0951	209
EP MC6 HV	W2 69-0937	203
EP MC6 HV	W2 69-0941	203
EP MC6 HV	W2 69-0945	203
EP MC6 LV	W2 69-0936	203
EP MC6 LV	W2 69-0940	203
EP MC6 LV	W2 69-0944	203
ESP/W-F10N	W2 64-0964	157, 159
ESP/W-F12N	W2 64-0965	157, 159
ESP/W-F15N	W2 64-0966	157, 159
ESP/W-F20N	W2 64-0967	157, 159
ESW-F10V	W2 64-1007	153
ESW-F12V	W2 64-1008	153
ESW-F15V	W2 64-1009	153
ESW-F20V	W2 64-1010	153
FC 100	W2 69-3023	283
FC-0	W2 64-0062	140
FC-1	W2 64-0063	140
FC-2	W2 64-0064	140
FR-50	W2 64-0220	84, 88, 106
FR-55S	W2 64-0221	84, 88, 106
FSW	W2 69-0157	305
G100-3	W2 64-0765	214
G100-4	W2 64-0766	214
G100-6	W2 64-0767	214
G100F-3	W2 64-0786	214
G100F-4	W2 64-0787	214
G100F-6	W2 64-0788	214
G100T-3	W2 64-0777	214
G100T-4	W2 64-0778	214
G100T-6	W2 64-0779	214
G100TF-3	W2 64-0798	215
G100TF-4	W2 64-0799	215
G100TF-6	W2 64-0800	215
G120-3	W2 64-0768	214
G120-4	W2 64-0769	214
G120-6	W2 64-0770	214
G120F-3	W2 64-0789	214
G120F-4	W2 64-0790	214
G120F-6	W2 64-0791	214
G120T-3	W2 64-0780	214
G120T-4	W2 64-0781	214
G120T-6	W2 64-0782	214
G120TF-3	W2 64-0801	215
G120TF-4	W2 64-0802	215
G120TF-6	W2 64-0803	215
G150-3	W2 64-0771	214
G150-4	W2 64-0772	214
G150-6	W2 64-0773	214
G150F-3	W2 64-0792	214
G150F-4	W2 64-0793	214
G150F-6	W2 64-0794	214
G150T-3	W2 64-0783	214
G150T-4	W2 64-0784	214
G150T-6	W2 64-0785	214
G150TF-3	W2 64-0804	215
G150TF-4	W2 64-0805	215
G150TF-6	W2 64-0806	215
G200-3	W2 64-0774	214
G200-4	W2 64-0775	214
G200-6	W2 64-0776	214
G200F-3	W2 64-0795	214
G200F-4	W2 64-0796	214
G200F-6	W2 64-0797	214
G200TF-3	W2 64-0807	215
G200TF-4	W2 64-0808	215
G200TF-6	W2 64-0809	215
G75150S-4	W2 64-0812	216
G75150T-4	W2 64-0813	216
G75165T-4	W2 64-0814	216
G85150T-3	W2 64-0817	216
G85150T-4	W2 64-0818	216
G85165T-3	W2 64-0819	216
G85165T-4	W2 64-0820	216
G86150T-4	W2 64-0815	216
G86165T-4	W2 64-0816	216
GBM10	W2 64-1587	85
GBM60	W2 64-1588	85
GH-1	W2 64-0124	81
GH-10	W2 64-0126	81
GH-2T	W2 64-0125	81
GR-36	W2 64-1459-36	258
GR-48	W2 64-1459-48	258
GR-60	W2 64-1459-60	258
GR-72	W2 64-1459-72	258
GS-30B/10	W2 64-0334	43
GS-30B/15	W2 64-0335	43
GS-30B/4	W2 64-0341	43
GS-30L/10	W2 64-0330	43
GS-30L/15	W2 64-0331	43
GS-30L/4	W2 64-0342	43
GS-30S/10	W2 64-0332	43
GS-30S/15	W2 64-0333	43
GS-30S/4	W2 64-0343	43

Warner Model Number Index

Warner Model	Order #	Page No.
HC-202B	W2 64-0005	133
HCS-1	W2 64-1543	126
HCS-RPL	W2 64-1544	126
HH-1	W2 64-0422	146
HM-507	W2 64-0080	137
HM-507	W2 64-0080	149
HOLD-1	W2 69-0165	305
HOLD-4	W2 69-0166	305
HOLD-7	W2 69-0167	305
HSC-1	W2 64-1543	115
HSC-1	W2 64-0543	116
IC-2S	W2 64-0046	160
IC-4M	W2 64-0047	160
IE-210	W2 64-0039	159
IE-251A	W2 64-0090	157
IP-1	W2 69-0154	305
JC-1	W2 64-1589	91
JC-1	W2 64-1589	92
JG-23N/HP	W2 64-1486	18
JG-23W/HP	W2 64-1487	18
JG-23W/LP	W2 64-1488	18
KS-1	W2 64-0081	140
KS-2	W2 64-0082	140
LC-201B	W2 64-0004	133
LPE-10	W2 64-1428	69, 79
LPE-50	W2 64-0141	86
LPF-100B	W2 64-0048	163
LPF-202A	W2 64-0049	163
LPF-8	W2 64-0050	143, 162
LU-ASP	W2 65-0047	121-123
LU-CB1	W2 65-0040	121
LU-CPC-CEH	W2 65-0041	122
LU-CPC-P	W2 65-0071	121-123
LU-CSD	W2 65-0049	117
LU-FPL	W2 65-0064	121-123
LU-FPZ	W2 65-0065	121-123
LU-PD	W2 65-0054	123
MAG-1	W2 64-0358	59
MAG-13	W2 64-0420	137
MAG-2	W2 64-0359	32, 59
MAG-22	W2 64-0421	137
MAG-3	W2 64-0360	59, 119
MAG-4	W2 64-0361	59
MAG-5	W2 64-1552	69
MAG-6	W2 64-1553	69
MAG-7	W2 64-1554	69
MAT-1	W2 64-1522	91, 92
MAT-2	W2 64-1523	78, 91, 92
MB/B	W2 64-0060	102, 146, 156
MC 100	W2 69-3016	282
MC-01G	W2 64-0019	135
MC-100M	W2 64-0020	135
MC-10G	W2 64-0018	135
MC-10GB	W2 64-0021	135
MC2-MO	W2 69-0935	202
MCK-1	W2 64-0357	59, 124, 125
MF-11	W2 69-0394	225
MF-1-115	W2 69-0384	225
MF-12	W2 69-0395	225
MF-1-230	W2 69-0438	225
MF-2	W2 69-0385	225
MF-3	W2 64-1610	226
MF-3E	W2 64-1614	226
MF-4	W2 69-0387	225
MF-5	W2 69-0388	225
MF-6	W2 69-0389	225
MF-7	W2 69-0390	225
MF-8	W2 69-0391	225
MF-9	W2 69-0392	225
MFG-3	W2 64-1612	226
MFG-3A	W2 64-1613	226
MFG-3AE	W2 64-1617	226
MFG-3E	W2 64-1616	226
MG-3	W2 64-1611	226
MG-3E	W2 64-1615	226
MHH-25	W2 64-0218	88, 242
MHH-38	W2 64-0219	88, 242
MI-M	W2 65-0052	118, 120-123
MI-T	W2 65-0070	123
ML-2	W2 64-0200	87
ML-4	W2 64-0201	87
ML-6	W2 64-0202	87
ML-8	W2 64-0199	87, 103
MM-2	W2 64-0203	87
MM-33L	W2 64-0055	156
MM-33R	W2 64-0056	156
MM-4	W2 64-0204	87
MM-6	W2 64-0205	87
MP-2	W2 64-0206	12, 13, 87
MP-3	W2 64-0207	12, 13, 87
MP-4	W2 64-0208	12, 13, 87
MP-5	W2 64-0209	12, 13, 84, 87
MP-6	W2 64-0210	12, 13, 87, 106
MP-8	W2 64-0211	12, 13, 87, 103
MPP-2	W2 64-0212	87
MPP-24	W2 64-0339	87
MPP-3	W2 64-0213	87
MPP-4	W2 64-0214	87
MPP-5	W2 64-0215	87
MPP-6	W2 64-0216	87
MPP-8	W2 64-0217	87
MS-7MT	W2 65-0208	220
MS-7PB	W2 65-0207	220
MSC-PTD	W2 65-0050	117
MSC-TD	W2 65-0051	117
MSH/10	W2 64-0152	83
MSH/10M	W2 64-0146	83
MSH/140	W2 64-0156	83
MSH/140M	W2 64-0150	83
MSH/20	W2 64-0153	83
MSH/20M	W2 64-0147	83
MSH/30	W2 64-0154	83
MSH/30M	W2 64-0148	83
MSH/5	W2 64-0151	83
MSH/5M	W2 64-0145	83
MSH/60	W2 64-0155	83
MSH/60M	W2 64-0149	83
MT200	W2 69-3033	280
MT200A	W2 72-6186	280
NL04	W2 65-0638	169
NL08	W2 65-0396	168
NL100AK	W2 65-0220	168
NL100RK	W2 65-0642	169
NL101A	W2 65-0221	169
NL101A	W2 65-0389	169
NL101A	W2 65-0390	169
NL101A	W2 65-0391	169
NL101B	W2 65-0392	169
NL101B	W2 65-0393	169
NL101B	W2 65-0394	169
NL101B	W2 65-0395	169
NL102G	W2 65-0222	167
NL102GH	W2 65-0223	167
NL104A	W2 65-0224	168
NL106	W2 65-0225	170
NL108A	W2 65-0227	171
NL108L2	W2 65-0231	172
NL108L4	W2 65-0631	171
NL108T2	W2 65-0229	172
NL108T2/10	W2 65-0230	172
NL108T4	W2 72-4222	171
NL120S	W2 65-0236	172
NL125/6	W2 65-0237	173
NL134	W2 65-0239	173
NL135	W2 65-0240	173
NL136	W2 65-0241	173
NL143	W2 65-0643	174
NL144	W2 65-0242	173
NL201	W2 65-0243	174
NL202	W2 65-0244	175
NL301	W2 65-0247	175
NL405	W2 65-0630	176, 177
NL410	W2 65-0252	176
NL412	W2 72-4220	178
NL50	W2 65-0219	165
NL501	W2 65-0253	179

Warner Model Number Index

Warner Model	Order #	Page No.
NL505	W2 65-0254	180
NL506	W2 65-0255	180
NL510A	W2 65-0256	181
NL512	W2 72-4221	182
NL530	W2 65-0259	181
NL601	W2 65-0260	183
NL603	W2 65-0261	183
NL703	W2 65-0266	184
NL800A	W2 65-0276	184
NL800BATT	W2 65-0363	184, 186
NL900D	W2 65-0283	164
NL905	W2 65-0283S	164
NL910D-1	W2 65-0632	186
NL910D-2	W2 65-0633	186
NL910D-4	W2 65-0634	186
NL910D-6	W2 65-0635	186
NL910D-8	W2 65-0636	186
NL911D-1	W2 65-0637	186
NL912-1	W2 65-0319	186
NL944	W2 65-0301	186
NL944K	W2 65-0302	186
NL950	W2 65-0289	186
NL951-15cm	W2 65-0386	186
NL951-1m	W2 65-0284	186
NL951-2m	W2 65-0385	186
NL951-30cm	W2 65-0387	186
NL951-45cm	W2 65-0388	186
NL952	W2 65-0285	186
NL953	W2 65-0286	186
NL953K	W2 65-0287	186
NL954	W2 65-0290	186
NL954K	W2 65-0291	186
NL955	W2 65-0292	186
NL955K	W2 65-0293	186
NL956K	W2 65-0294	186
NL957	W2 65-0308	186
NL957K	W2 65-0309	186
NL960	W2 65-0310	186
NL961	W2 65-0311	186
NL962	W2 65-0295	186
NL963	W2 65-0296	186
NL963K	W2 65-0297	186
NL964	W2 65-0303	186
NL965	W2 65-0305	186
NL965K	W2 65-0306	186
NL966K	W2 65-0307	186
NL967K	W2 65-0298	186
NL968K	W2 65-0299	186
NL969P	W2 65-0300	186
NL969S	W2 65-0304	186
NL969T	W2 65-0312	186
NL970/10	W2 65-0320	186
NL972/10	W2 65-0321	186
NL973A	W2 65-0313	186
NL975	W2 65-0288	186
NL976	W2 65-0314	186
NL980	W2 65-0322	186
NL985	W2 65-0323	172
NL985	W2 65-0323	186
NLMAN	W2 65-0325	186
NYL/MESH	W2 64-0198	67
OC-725C	W2 64-0028	153, 156
ON-750A	W2 64-0069	137
ON-750A-EU	W2 64-0073	149
ON-750A-US	W2 64-0069	149
OP-1	W2 69-0155	305
OP-2	W2 69-0156	305
OS-250	W2 64-1520	91
OW-24/20.3M	W2 64-1480M	105
OW-24/25M	W2 64-1479M	105
OW-26/20.3M	W2 64-1478M	105
OW-26/25M	W2 64-1477M	105
OW-28/20.3M	W2 64-1476M	105
OW-28/25M	W2 64-1475M	105
OW-29/20.3M	W2 64-1474M	105
OW-29/25M	W2 64-1473M	105
OW-30/20.3M	W2 64-1472M	105
OW-30/25M	W2 64-1471M	105
OW-32/20.3M	W2 64-1470M	105
OW-32/25M	W2 64-1469M	105
OW-33.5/20.3M	W2 64-1468M	105
OW-33.5/25M	W2 64-1467M	105
OW-34/20.3M	W2 64-1466M	105
OW-34/25M	W2 64-1465M	105
OW-39/20.3M	W2 64-1594	105
OW-39/25M	W2 64-1593	105
P-1	W2 64-0277	18, 25-27, 29, 31, 33
P-1	W2 64-0277	55
P-2	W2 64-0278	20-23, 55
P2000	W2 69-0997	205
P2020	W2 69-0987	205
P2020-I	W2 69-0989	205
P2020-V	W2 69-0988	205
P2023-100	W2 69-0992	205
P2023-20	W2 69-0990	205
P2023-50	W2 69-0991	205
P2024	W2 69-0998	205
P2300	W2 69-0993	205
P2302	W2 69-0956	205
P2304	W2 69-0957	205
P2305	W2 69-0958	205
P2306	W2 69-0959	205
P2307	W2 69-0960	205
P2310	W2 69-0961	205
P2311	W2 69-0962	205
P2312	W2 69-0963	205
P2313	W2 69-0964	205
P2314	W2 69-0965	205
P2315	W2 69-0966	205
P2404	W2 69-0969	205
P2405	W2 69-0970	205
P2406	W2 69-0971	205
P2407	W2 69-0972	205
P2410	W2 69-0973	205
P2411	W2 69-0974	205
P2412	W2 69-0975	205
P2413	W2 69-0976	205
P-3	W2 64-0279	28, 55
P-4	W2 64-0280	28
P-4	W2 64-0280	55
P-5	W2 64-0281	19
P-5	W2 64-0281	55
P-6	W2 64-0282	34, 37-39
P-6	W2 64-0282	55
P-6D	W2 64-0283	36, 40
P-6D	W2 64-0283	55
PA2	W2 64-1460	258
PAC	W2 64-1462	258
PC-501A/10	W2 64-0007	135
PC-501A/10B	W2 64-0010	135
PC-501A/8	W2 64-0009	135
PC-501A/9	W2 64-0008	135
PC-501AV/8	W2 64-0013	135
PC-501AV/9	W2 64-0012	135
PC-505BHB	W2 64-0002	133
PC-505BHC	W2 64-0001	133
PC-505BLC	W2 64-0000	133
PDMI-2	W2 65-0043	117
PDMI-ARL	W2 65-0093	123
PDMI-ARN	W2 65-0059	123
PDMI-ARO	W2 65-0060	123
PDMI-ARZ	W2 65-0061	123
PDMI-FPL	W2 65-0062	123
PDMI-FPZ	W2 65-0063	123
PDMI-TUBE	W2 65-0058	123
PE-10/10	W2 64-0750	70, 81, 86
PE-10/100	W2 64-0751	70
PE-160/10	W2 64-0755	12, 13, 18-23, 25-29, 31-34, 36-40, 50, 51, 53, 70, 79, 84, 86, 102, 103, 106
PE-160/100	W2 64-0756	70, 79, 84
PE-50/10	W2 64-0752	70, 79, 81, 85, 86, 103
PE-50/100	W2 64-0753	70, 79, 85
PE-90/10	W2 64-0754	50, 53, 70, 79, 86

Warner Model Number Index

Warner Model	Order #	Page No.
PH-1	W2 64-0284	18, 25-27, 29, 31, 33, 55
PH-2	W2 64-0285	20-23, 55
PH-3	W2 64-0286	28, 55
PH-4	W2 64-0287	28
PH-4	W2 64-0287	55
PH-5	W2 64-0288	19
PH-5	W2 64-0288	55
PH-6	W2 64-0289	34, 37, 38, 39
PH-6	W2 64-0289	55
PH-6D	W2 64-0290	36, 40
PH-6D	W2 64-0290	55
PHC-1	W2 64-0354	104
PHC-2	W2 64-0355	104
PHC-3	W2 64-0356	104
PI-1	W2 64-0180	111
PJ1-10	W2 64-1322	295
PJ2-5	W2 64-1323	69, 161, 295
PLI-100	W2 65-0001	301
PLI-100 Deluxe	W2 65-0003	301
PLI-100 Plus	W2 65-0002	299, 301
PLI-90 Basic	W2 65-0004	302
PLI-90 Plus	W2 65-0005	302
PLI-FS	W2 65-0029	303
PLI-HHN	W2 65-0012	303
PLI-HHO	W2 65-0011	303
PLI-HN	W2 65-0020	303
PLI-IHA	W2 65-0006	303
PLI-IHN	W2 65-0008	303
PLI-IHO	W2 65-0007	303
PLI-OHN	W2 65-0010	303
PLI-OHO	W2 65-0009	303
PLI-PC	W2 65-0019	303
PLI-PH1	W2 65-0013	303
PLI-PH1A	W2 65-0014	303
PLI-PHA	W2 65-0022	303
PLI-PH-KIT	W2 65-0021	303
PLI-PPH	W2 65-0023	303
PLI-RM	W2 65-0030	303
PLI-SRG	W2 65-0017	303
PLI-SRG1.5	W2 65-0015	303
PLI-SSB	W2 65-0018	303
PLS-1	W2 64-1608	299
PM-1	W2 64-1526	18, 25-27, 29, 31, 33, 57
PM-2	W2 64-1561	20-23, 57
PM-3	W2 64-1562	28, 57
PM-4	W2 64-1563	28, 57
PM-5	W2 64-1564	19, 57
PM-6	W2 64-1527	34, 37-39, 57
PM-6D	W2 64-1528	36, 40, 57
PM-7	W2 64-1529	35, 57
PM-7D	W2 64-1532	35
PM-7D	W2 64-1530	57
PM-8	W2 64-1531	32, 57
PM-KP	W2 69-0158	305
PP-4	W2 69-0164	305
PP-7	W2 69-0163	305
PS-560	W2 64-0182	107, 108, 111
PS-CSD	W2 65-0053	118, 123
PSMI	W2 65-0044	118
PT-QE1	W2 64-1404	68, 124
PV-1	W2 64-0139	79
QE-1	W2 64-0375	46, 47, 49-51, 124
QE-2	W2 64-1542	54, 125
QSW-A10P	W2 64-0821	133, 135
QSW-A12P	W2 64-0822	133, 135
QSW-A15P	W2 64-0823	133, 135
QSW-A17P	W2 64-0978	133, 135
QSW-A20P	W2 64-0824	133, 135
R-3603	W2 72-1015	89
RAC-14	W2 64-0070	146
RB-1	W2 64-0041	159
RC 300	W2 69-3018	282
RC 350	W2 69-3019	282
RC 650	W2 69-3021	281
RC-10	W2 64-0306	14
RC-11	W2 64-0307	14
RC-13	W2 64-0308	14
RC-16	W2 64-0309	14
RC-1Z	W2 64-0318	12
RC-20	W2 64-0222	19
RC-20H	W2 64-0223	19
RC-21B	W2 64-0224	20
RC-21BDW	W2 64-0362	22
RC-21BR	W2 64-0225	20
RC-21BRFS	W2 64-0226	21
RC-21BRW	W2 64-0227	23
RC-22	W2 64-0228	25
RC-22C	W2 64-0229	25
RC-24	W2 64-0230	26
RC-24E	W2 64-0231	26
RC-24N	W2 64-0381	27
RC-25	W2 64-0232	28
RC-25F	W2 64-0233	28
RC-26	W2 64-0234	31
RC-26G	W2 64-0235	31
RC-26GLP	W2 64-0236	29
RC-26GS	W2 64-1534	32
RC-26Z	W2 64-0237	33
RC-27	W2 64-0238	34
RC-27D	W2 64-1548	35
RC-27L	W2 64-0241	36
RC-27LD	W2 64-1532	35
RC-27N	W2 64-0239	37
RC-27NE	W2 64-0240	38
RC-28	W2 64-0243	39
RC-29	W2 64-0244	40
RC-30	W2 64-0320	43
RC-30HV	W2 64-0321	43
RC30TCP	W2 64-1464	43
RC30TCPWA	W2 64-1464WA	43
RC-30WA	W2 64-0321WA	43
RC-33DL	W2 64-1482	44
RC-33DM	W2 64-1481	44
RC-33Kit	W2 64-1485	44
RC-33SM	W2 64-1484	44
RC-33SN	W2 64-1483	44
RC-37F	W2 64-0348	45
RC-37FC	W2 64-0364	46
RC-37FS	W2 64-0366	47
RC-37W	W2 64-0347	45
RC-37WC	W2 64-0363	46
RC-37WS	W2 64-0365	47
RC-3Z	W2 64-0319	13, 156
RC-4	W2 64-1458	258
RC-40HP	W2 64-0370	50
RC-40LP	W2 64-0367	49
RC-41LP	W2 64-0368	49
RC-42LP	W2 64-0369	49
RC-43C	W2 64-0371	50
RC-46SLP	W2 64-0372	51
RC-46SNLP	W2 64-0373	51
RC-47FSLP	W2 64-0374	51
RC-48LP	W2 64-0387	49
RC-50	W2 64-0605	53
RC-50-D15X10	W2 64-0610	53
RC-50-R15	W2 64-0607	53
RC-50-R3	W2 64-0606	53
RC-50-S2.5X10	W2 64-0609	53
RC-50-S3X7	W2 64-0608	53
RC-61T-01	W2 64-1535	54
RC-61T-02	W2 64-1536	54
RC-61T-03	W2 64-1537	54
RC-61T-04	W2 64-1538	54
RC-61T-05	W2 64-1539	54
RC-61T-06	W2 64-1540	54
RC-61T-Kit	W2 64-1541	54
REF-1L	W2 64-1301	294
REF-2L	W2 64-1302	294
REF-3L	W2 64-1303	294
RH-2	W2 64-0274	19, 58
RH-3	W2 64-1559	43
RK-2	W2 69-0160	305
RPC-1	W2 64-1506	58

Warner Model Number Index

Warner Model	Order #	Page No.
RPC-2	W2 64-1507	58, 126
RS-1	W2 64-0162	79, 83, 84, 106, 107
SA-20LZ	W2 64-0296	114
SA-30/OLY2	W2 64-0325	43
SA-30/OLY2	W2 64-0325	53
SA-30GALVOZ	W2 64-0377	43
SA-30GALVOZ	W2 64-0377	53
SA-30GALVZi	W2 64-1456	43
SA-30GALZi	W2 64-1456	53
SA-30KZ	W2 64-0327	43
SA-30KZ	W2 64-0327	53
SA-30L3P	W2 64-0328	43
SA-30L3P	W2 64-0328	53
SA-30LZ	W2 64-0326	43
SA-30LZ	W2 64-0326	53
SA-30NIK	W2 64-0322	43
SA-30NIK	W2 64-0322	53
SA-30PLI	W2 64-0329	43
SA-30PLI	W2 64-0329	53
SA-30TMS/9	W2 64-0324	43
SA-30TMS9	W2 64-0324	53
SA-30UU	W2 64-0380	43
SA-30UU	W2 64-0380	53
SA-30UUZ	W2 64-0379	43
SA-30UUZ	W2 64-0379	53
SA-NIK	W2 64-0291	114
SA-OLY/2	W2 64-0295	114
SC-20	W2 64-0353	96, 101
SDR	W2 64-1607	258
SF-28	W2 64-0103	100, 115, 116, 119, 124
SF-77B	W2 64-0114	81
SF-77B	W2 64-1515	81
SF-77B/5M	W2 64-0117	81
SF-77B/5M	W2 64-1518	81
SF-77BLT	W2 64-0116	81
SF-77BLT	W2 64-1517	81
SF-77BST	W2 64-0115	81
SF-77BST	W2 64-1516	81
SG-1000-5	W2 64-0122	81
SG-800-5	W2 64-0121	81
SH-27B	W2 64-0102	100, 115, 116, 119, 124, 125
SH-27G	W2 64-1503	100
SH2CO	W2 64-0382	90
SH-6/140	W2 64-0144	79, 83
SH-6/60	W2 64-0163	79, 83
SH-8/10	W2 64-0143	79, 83
SH-8/60	W2 64-0385	79, 83
SHD-22CF/10	W2 64-1414	66
SHD-22CF/15	W2 64-1413	66
SHD-22CKit	W2 64-0264	25, 67
SHD-22CL/10	W2 64-0249	66
SHD-22CL/15	W2 64-0247	25, 66
SHD-22F/10	W2 64-1412	66
SHD-22Kit	W2 64-0263	25, 67
SHD-22L/10	W2 64-0248	66
SHD-22L/15	W2 64-0246	25, 66
SHD-26GH/10	W2 64-0253	18, 31, 66
SHD-26GH/15	W2 64-0254	18, 31, 66
SHD-26GH/2	W2 64-0255	66
SHD-26GH/20	W2 64-0255	18, 31
SHD-26GH2	W2 64-0255	29
SHD-26GKIT	W2 64-0266	67
SHD-26H/10	W2 64-0253	29
SHD-26H/10	W2 64-0250	31, 66
SHD-26H/15	W2 64-0254	29
SHD-26H/15	W2 64-0251	31, 66
SHD-26H/2	W2 64-0252	66
SHD-26H/20	W2 64-0252	31
SHD-26KIT	W2 64-0265	67
SHD-27H/10	W2 64-0194	34, 66
SHD-27H/15	W2 64-0193	34, 66
SHD-27H/2	W2 64-0192	66
SHD-27H/20	W2 64-0192	34
SHD-27KIT	W2 64-0267	34, 67
SHD-27LH/10	W2 64-0256	35, 36, 40, 66
SHD-27LH/15	W2 64-0257	35, 36, 40, 66
SHD-27LH/2	W2 64-0258	66
SHD-27LH/20	W2 64-0258	35, 36, 40
SHD-27LKIT	W2 64-0268	36, 67
SHD-27LP/10	W2 64-0259	35, 36, 40, 66
SHD-27LP/15	W2 64-0260	35, 36, 40, 66
SHD-27LP/2	W2 64-0261	66
SHD-27LP/20	W2 64-0261	35, 36, 40
SHD-27LPKIT	W2 64-0190	36, 67
SHD-27N/10	W2 64-0197	37, 66
SHD-27N/15	W2 64-0196	37, 66
SHD-27N/20	W2 64-0195	37, 66
SHD-27NKIT	W2 64-0191	37, 67
SHD-40/10	W2 64-1417	66
SHD-40/15	W2 64-1416	66
SHD-40/2	W2 64-1415	66
SHD-41/10	W2 64-1419	66
SHD-41/15	W2 64-1418	66
SHD-42/10	W2 64-1421	66
SHD-42/15	W2 64-1420	66
SHH-1	W2 64-1555	110
SHH-2	W2 64-1556	110
SHH-3	W2 64-1557	110
SHH-4	W2 64-1558	110
SHM-6	W2 64-0104	102
SHM-8	W2 64-0105	102
SHM-828	W2 64-1430	96, 103
SIU-102	W2 64-1424	47, 51, 210
SK205	W2 72-6187	280
SK206	W2 72-6188	280
SL2CO	W2 64-0383	90
SL-6	W2 64-0165	79, 83, 84, 106, 107, 189
SL-6U	W2 64-0567	189
SLAM 05N	W2 64-1600	308
SLAM 05Ω	W2 64-1602	308
SLAM 10N	W2 64-1601	308
SLAM 10Ω	W2 64-1603	308
SN-18	W2 64-1489	79, 86
SN-23	W2 64-1490	79, 86
SN-30	W2 64-1583	86
SPIN-2	W2 64-0074	145
SS-3	W2 64-0273	19
SS-10	W2 64-1461-10	258
SS-12	W2 64-1461-12	258
SS-14	W2 64-1461-14	258
SS-3	W2 64-0273	36, 40
SS-3G	W2 64-1533	67
SS-4-500H	W2 64-1551	35, 67
SS-4-500V	W2 64-1550	35, 67
ST-1	W2 64-0272	19
ST-1L	W2 64-1401	68
ST-1R	W2 64-1400	68
ST-1S	W2 64-1431	68
ST-1Z	W2 64-1402	68
ST-3	W2 64-1406	32, 68
ST-37	W2 64-1405	68
ST-3L	W2 64-1408	68
ST-3R	W2 64-1407	68
ST-4	W2 64-1409	68
ST-5	W2 64-1410	68
ST-QE1	W2 64-1403	68, 124, 125
STU-1	W2 64-1429	58, 70
SUN-1	W2 64-0061	145
SUN-DCH	W2 64-0065	145
SUNSTIR	W2 64-0075	145
SUNSTIR-3	W2 64-0076	145
SV-1	W2 64-0175	79
SW-10/6	W2 64-0111	106
SW-60	W2 64-0179	108
SW-61	W2 64-0112	107
SW-707	W2 64-0181	108
SWS-10	W2 64-1584	109
SWS-140	W2 64-1585	109
SWS-60	W2 64-1560	109
TA-29	W2 64-0107	58, 96, 100-103, 110
TA-30	W2 64-0108	58, 100, 102, 103, 110

Warner Model Number Index

Warner Model	Order #	Page No.
TC-124	W2 64-1545	98, 105, 109
TC-124E	W2 64-1545E	98, 105, 109
TC-202A	W2 65-0045	97, 120, 121, 122, 129
TC-3	W2 64-0164	79
TC-324B	W2 64-0100	95, 100, 102, 115, 116, 119, 124, 125, 129
TC-324BHT	W2 64-1453	95
TC-344B	W2 64-0101	95, 100, 102, 115, 116, 119, 124, 125, 129
TC-344BHT	W2 64-1454	95
TC-CA	W2 65-0072	121-123
TEV700	W2 64-0034	156
TG150-4	W2 64-0810	215
TG200-4	W2 64-0811	81, 215
TJ1-3	W2 64-1324	295
TS-30G	W2 64-0271	19
TS-60P	W2 64-0269	19, 58
TS-70B	W2 64-0270	19, 58
TT-25	W2 64-0168	79
TV-2	W2 64-0140	79
TY-50	W2 64-0167	79
U2500/A	W2 64-0575	191
U2500/B	W2 64-0576	191
U2500/C	W2 64-0577	191
U2500/F	W2 64-0578	191
U2500/M	W2 64-0579	191
U2500/S	W2 64-0580	191
U2500/T	W2 64-0581	191
U9302	W2 64-0560	189
U9303	W2 64-0561	189
U9304	W2 64-0556	189
U9310	W2 64-0557	189
U9320	W2 64-0558	189
U9403	W2 64-0562	189
U9403R	W2 64-0563	189
U9404	W2 64-0564	102, 189
U9406	W2 64-0565	191
U9500	W2 64-0500	189
U9500DR	W2 64-0501	189
U9500S	W2 64-0502	189
U9500SDR	W2 64-0503	189
U9504	W2 64-0504	189
U9504SP-1	W2 64-0509	189
U9504SP-2	W2 64-0510	189
U9504SP-3	W2 64-0511	189
U9506	W2 64-0505	189
U9509	W2 64-0506	189
U9512	W2 64-0507	189
U9513	W2 64-0508	189
U9520/A	W2 64-0520	189
U9520/B	W2 64-0521	189
U9520/F	W2 64-0522	189
U9520/M	W2 64-0523	189
U9520/S	W2 64-0524	189
U9520/T	W2 64-0525	189
U9521	W2 64-0532	189
U9521DR	W2 64-0533	189
U9524A-04	W2 64-0534	189
U9524A-06	W2 64-0535	189
U9524A-09	W2 64-0536	189
U9524A-12	W2 64-0537	189
U9524A-12	W2 64-0538	189
U9524B-04	W2 64-0539	189
U9524B-06	W2 64-0540	189
U9524B-09	W2 64-0541	189
U9524B-12	W2 64-0542	189
U9524B-13	W2 64-0543	189
U9524F-09	W2 64-0544	189
U9524F-12	W2 64-0545	189
U9524F-25	W2 64-0546	189
U9524M-12	W2 64-0547	189
U9524M-30	W2 64-0548	189
U9524S	W2 64-0549	189
U9524T-06	W2 64-0550	189
U9524T-12	W2 64-0551	189
U9524T-24	W2 64-0552	189
U9565EP	W2 64-0553	189, 191
U9924A-04	W2 64-0582	191
U9924A-06	W2 64-0583	191
U9924A-09	W2 64-0584	191
U9924A-12	W2 64-0585	191
U9924A-13	W2 64-0586	191
U9924B-04	W2 64-0587	191
U9924B-06	W2 64-0588	191
U9924B-09	W2 64-0589	191
U9924B-12	W2 64-0590	191
U9924B-13	W2 64-0591	191
U9924C-03	W2 64-0592	191
U9924C-04	W2 64-0593	191
U9924C-05	W2 64-0594	191
U9924F-09	W2 64-0595	191
U9924F-12	W2 64-0596	191
U9924F-25	W2 64-0597	191
U9924M-30	W2 64-0599	191
U9924S	W2 64-0600	191
U9924T-06	W2 64-0601	191
U9924T-12	W2 64-0602	191
U9924T-24	W2 64-0603	191
U9926/A	W2 64-0568	191
U9926/B	W2 64-0569	191
U9926/C	W2 64-0570	191
U9926/F	W2 64-0571	191
U9926/M	W2 64-0572	191
U9926/S	W2 64-0573	191
U9926/T	W2 64-0574	191
U9975A	W2 64-0554	189, 191
U9985	W2 64-0555	189, 191
VC-64CS	W2 64-0134	77
VC-66BB	W2 64-0129	77
VC-66BBT	W2 64-0132	77
VC-66CS	W2 64-0135	77
VC-66CST	W2 64-0138	77
VC-66MBB	W2 64-0171	77
VC-66MCS	W2 64-0174	77
VC-77SP	W2 64-0177	82
VC-77SP	W2 64-1519	82
VC-77SP8	W2 64-1590	82
VC-77SP8E	W2 64-1590E	82
VC-77SPL	W2 64-0177L	82
VC-77SPLE	W2 64-177LE	82
VC-8M	W2 64-0186	78
VC-8MLT	W2 64-0186LT	78
VC-8P	W2 64-0185	78
VC-8T	W2 64-0187	78
VCC MC2	W2 69-0933	202
VCC MC2-HV	W2 69-0934	202
VCC MC8 HV	W2 69-1005	203
VCC MC8 LV	W2 69-1003	203
VCC600	W2 69-0930	199
VCC600HV	W2 69-0931	199
W6-205B	W2 64-0006	133
WA10-5	W2 64-1327	295
WA30-5	W2 64-1328	295
WC1-10	W2 64-1325	295
WC2-5	W2 64-1326	295
WIS-1-R	W2 69-0117	99
ZM-186	W2 64-0071	137
ZM-186	W2 64-0071	149

Ordering Number Index

Order #	Page No.
W2 30-0001	219
W2 30-0002	219
W2 30-0003	219
W2 30-0004	218
W2 30-0005	218
W2 30-0006	218
W2 30-0007	219
W2 30-0008	219
W2 30-0012	219
W2 30-0013	219
W2 30-0014	219
W2 30-0015	219
W2 30-0016	217
W2 30-0017	217
W2 30-0018	217
W2 30-0019	218
W2 30-0020	218
W2 30-0021	218
W2 30-0032	218
W2 30-0033	218
W2 30-0034	218
W2 30-0035	217
W2 30-0036	217
W2 30-0037	217
W2 30-0038	218
W2 30-0039	218
W2 30-0040	218
W2 30-0041	217
W2 30-0042	217
W2 30-0043	217
W2 30-0044	218
W2 30-0045	218
W2 30-0046	218
W2 30-0047	217
W2 30-0048	217
W2 30-0049	217
W2 30-0050	218
W2 30-0051	218
W2 30-0052	218
W2 30-0053	217
W2 30-0054	217
W2 30-0055	217
W2 30-0056	217
W2 30-0057	218
W2 30-0058	218
W2 30-0060	218
W2 30-0062	217
W2 30-0063	217
W2 30-0064	217
W2 30-0065	217
W2 30-0066	218
W2 30-0067	218
W2 30-0068	218
W2 30-0070	217
W2 30-0071	217
W2 30-0073	217
W2 30-0074	218
W2 30-0075	218
W2 30-0076	218
W2 30-0077	218
W2 30-0078	218
W2 30-0080	217
W2 30-0081	217
W2 30-0082	218
W2 30-0083	218
W2 30-0084	218
W2 30-0085	219
W2 30-0086	219
W2 30-0087	219
W2 30-0089	216
W2 30-0090	216
W2 30-0091	216
W2 30-0092	216
W2 30-0093	216
W2 30-0094	216
W2 30-0095	216
W2 30-0096	216
W2 30-0097	216
W2 30-0108	219
W2 30-0109	219
W2 30-0110	219
W2 30-0114	218
W2 30-0115	218
W2 30-0116	218
W2 30-0117	218
W2 30-0118	218
W2 30-0119	218
W2 30-0127	217
W2 30-0128	218
W2 50-1932	277
W2 50-1940	277
W2 55-4148	74
W2 56-4930	272, 273
W2 56-5002	272, 273
W2 56-5028	272, 274
W2 56-5036	274
W2 56-5077	272, 274
W2 60-0569	244, 248
W2 60-0570	244, 248
W2 60-0571	245, 250, 299
W2 60-0572	245, 250
W2 60-0574	245, 250
W2 60-0577	251, 299
W2 60-0580	251
W2 60-0581	251
W2 60-0582	244, 252
W2 60-0583	244, 252
W2 60-0586	245, 253
W2 60-0588	245, 253
W2 60-0590	245, 253
W2 60-0592	245, 253
W2 60-0594	244, 253
W2 60-0600	245, 250
W2 60-0601	245, 250
W2 60-0604	248, 251-253
W2 61-0098	75
W2 61-0130	272
W2 61-0131	274
W2 61-0132	274
W2 61-0133	274
W2 61-0134	273
W2 61-0136	273
W2 61-0137	273
W2 61-0138	272, 274
W2 61-0139	274
W2 61-0140	274
W2 61-0239	75
W2 61-0241	75
W2 61-0242	75
W2 61-0243	75
W2 61-0244	75
W2 61-0245	75
W2 61-0247	274
W2 61-0248	272, 274
W2 61-0249	272, 274
W2 61-0250	274
W2 64-0000	133
W2 64-0001	133
W2 64-0002	133
W2 64-0004	133
W2 64-0005	133
W2 64-0006	133
W2 64-0007	135
W2 64-0008	135
W2 64-0009	135
W2 64-0010	135
W2 64-0012	135
W2 64-0013	135
W2 64-0014	135
W2 64-0015	135
W2 64-0016	135
W2 64-0017	135
W2 64-0018	135
W2 64-0019	135
W2 64-0020	135
W2 64-0021	135
W2 64-0024	137
W2 64-0024	148
W2 64-0025	148
W2 64-0026	137
W2 64-0026	148
W2 64-0027	148
W2 64-0028	153, 156
W2 64-0029	153
W2 64-0030	153
W2 64-0031	153
W2 64-0032	153
W2 64-0033	153
W2 64-0034	156
W2 64-0035	201
W2 64-0036	201
W2 64-0039	159
W2 64-0040	159
W2 64-0041	159
W2 64-0042	159
W2 64-0043	157
W2 64-0044	160
W2 64-0045	160
W2 64-0046	160
W2 64-0047	160
W2 64-0048	163
W2 64-0049	163
W2 64-0050	143, 162
W2 64-0055	156
W2 64-0055	244, 248
W2 64-0056	156
W2 64-0056	244, 248
W2 64-0057	248
W2 64-0058	248
W2 64-0060	102, 146, 156
W2 64-0060	299
W2 64-0061	145
W2 64-0062	140
W2 64-0063	140
W2 64-0064	140
W2 64-0065	145
W2 64-0067	146
W2 64-0069	123
W2 64-0069	137
W2 64-0069	149
W2 64-0070	146
W2 64-0071	137
W2 64-0071	149
W2 64-0073	149
W2 64-0074	145
W2 64-0075	145
W2 64-0076	145
W2 64-0077	150
W2 64-0078	137, 150
W2 64-0080	137
W2 64-0080	149
W2 64-0081	140
W2 64-0081	257
W2 64-0082	140
W2 64-0082	257
W2 64-0090	157
W2 64-0100	95, 100, 102, 115, 116, 119, 124, 125, 129
W2 64-0101	95, 100, 102, 115, 116, 119, 124, 125, 129
W2 64-0102	100, 115, 116, 119, 124, 125
W2 64-0103	100, 115, 116, 119, 124
W2 64-0104	102
W2 64-0105	102
W2 64-0106	58, 95, 110, 114-116, 119, 124, 125
W2 64-0107	58, 96, 100, 101-103, 110
W2 64-0108	58, 100, 102, 103, 110
W2 64-0109	58, 95, 110
W2 64-0110	46, 47, 114
W2 64-0111	106
W2 64-0112	107
W2 64-0114	81
W2 64-0115	81
W2 64-0116	81
W2 64-0117	81
W2 64-0119	81
W2 64-0120	81
W2 64-0121	81
W2 64-0122	81
W2 64-0124	81
W2 64-0125	81
W2 64-0126	81
W2 64-0129	77
W2 64-0132	77
W2 64-0134	77
W2 64-0135	77
W2 64-0138	77
W2 64-0139	79
W2 64-0140	79
W2 64-0141	86
W2 64-0142	79
W2 64-0143	79, 83
W2 64-0144	79, 83
W2 64-0145	83
W2 64-0146	83
W2 64-0146	84
W2 64-0147	83
W2 64-0147	84
W2 64-0148	83
W2 64-0149	83
W2 64-0149	84
W2 64-0150	83
W2 64-0150	84
W2 64-0151	83
W2 64-0152	83
W2 64-0152	84
W2 64-0153	83
W2 64-0153	84
W2 64-0154	83
W2 64-0155	83
W2 64-0155	84
W2 64-0156	83
W2 64-0156	84
W2 64-0157	84
W2 64-0158	84
W2 64-0159	84
W2 64-0160	84
W2 64-0161	84
W2 64-0162	79, 83, 84, 106, 107
W2 64-0163	79, 83
W2 64-0164	79
W2 64-0165	79, 83, 84, 106, 107, 189
W2 64-0166	79, 86
W2 64-0167	79
W2 64-0168	79
W2 64-0171	77
W2 64-0174	77
W2 64-0175	79
W2 64-0177	82
W2 64-0177L	82
W2 64-0179	108
W2 64-0180	111
W2 64-0181	108
W2 64-0182	107, 108, 111
W2 64-0185	78
W2 64-0186	78
W2 64-0186LT	78
W2 64-0187	78
W2 64-0190	36, 67
W2 64-0191	37, 67
W2 64-0192	66
W2 64-0192	34
W2 64-0193	34, 66
W2 64-0194	34, 66

Ordering Number Index

Order #	Page No.
W2 64-0195	37, 66
W2 64-0196	37, 66
W2 64-0197	37, 66
W2 64-0198	67
W2 64-0198	25
W2 64-0199	87, 103
W2 64-0200	87
W2 64-0201	87
W2 64-0202	87
W2 64-0203	87
W2 64-0204	87
W2 64-0205	87
W2 64-0206	12, 13, 87
W2 64-0207	12, 13, 87
W2 64-0208	12, 13, 87
W2 64-0209	12, 13, 84, 87
W2 64-0210	12, 13, 87, 106
W2 64-0211	12, 13, 87, 103
W2 64-0212	87
W2 64-0213	87
W2 64-0214	87
W2 64-0215	87
W2 64-0216	87
W2 64-0217	87
W2 64-0218	88, 242
W2 64-0219	88, 242
W2 64-0220	84, 88, 106
W2 64-0221	84, 88, 106
W2 64-0222	19
W2 64-0223	19
W2 64-0224	20
W2 64-0225	20
W2 64-0226	21
W2 64-0227	23
W2 64-0228	25
W2 64-0229	25
W2 64-0230	26
W2 64-0231	26
W2 64-0232	28
W2 64-0233	28
W2 64-0234	31
W2 64-0235	31
W2 64-0236	29
W2 64-0237	33
W2 64-0238	34
W2 64-0239	37
W2 64-0240	38
W2 64-0241	36
W2 64-0243	39
W2 64-0244	40
W2 64-0246	25, 66
W2 64-0247	25, 66
W2 64-0248	66
W2 64-0249	66
W2 64-0250	31, 66
W2 64-0251	31, 66
W2 64-0252	66
W2 64-0252	31
W2 64-0253	18, 31, 66
W2 64-0253	29
W2 64-0254	18, 31, 66
W2 64-0254	29
W2 64-0255	66
W2 64-0255	18, 31
W2 64-0255	29
W2 64-0256	35, 36, 40, 66
W2 64-0257	35, 36, 40, 66
W2 64-0258	66
W2 64-0258	35, 36, 40
W2 64-0259	35, 36, 40, 66
W2 64-0260	35, 36, 40, 66
W2 64-0261	66
W2 64-0261	35, 36, 40
W2 64-0263	25, 67
W2 64-0264	25, 67
W2 64-0265	67
W2 64-0266	67
W2 64-0267	34, 67
W2 64-0268	36, 67
W2 64-0269	19, 58
W2 64-0270	19, 58
W2 64-0271	19
W2 64-0272	19
W2 64-0273	19, 36, 40
W2 64-0274	19, 58
W2 64-0275	70
W2 64-0276	19, 58
W2 64-0277	18, 25-27, 29, 31, 33
W2 64-0277	55
W2 64-0278	20-23, 55
W2 64-0279	28, 55
W2 64-0280	28
W2 64-0280	55
W2 64-0281	19
W2 64-0281	55
W2 64-0282	34, 37-39
W2 64-0282	55
W2 64-0283	36, 40
W2 64-0283	55
W2 64-0284	18, 25-27, 29, 31, 33, 55
W2 64-0285	20-23, 55
W2 64-0286	28, 55
W2 64-0287	28
W2 64-0287	55
W2 64-0288	19
W2 64-0288	55
W2 64-0289	34, 37-39
W2 64-0289	55
W2 64-0290	36, 40
W2 64-0290	55
W2 64-0291	114
W2 64-0291	60
W2 64-0292	60
W2 64-0293	60
W2 64-0294	60
W2 64-0295	114
W2 64-0295	60
W2 64-0296	114
W2 64-0296	60
W2 64-0297	60
W2 64-0298	60
W2 64-0299	60
W2 64-0300	60
W2 64-0301	60
W2 64-0302	60, 318
W2 64-0303	58, 110
W2 64-0306	14
W2 64-0307	14
W2 64-0308	14
W2 64-0309	14
W2 64-0311	15
W2 64-0312	15
W2 64-0313	15
W2 64-0314	15
W2 64-0315	15
W2 64-0316	15
W2 64-0317	15
W2 64-0318	12
W2 64-0319	13, 156
W2 64-0320	43
W2 64-0321	43
W2 64-0321WA	43
W2 64-0322	43
W2 64-0322	53
W2 64-0324	43
W2 64-0324	53
W2 64-0325	43
W2 64-0325	53
W2 64-0326	43
W2 64-0326	53
W2 64-0327	43
W2 64-0327	53
W2 64-0328	43
W2 64-0328	53
W2 64-0329	43
W2 64-0329	53
W2 64-0330	43
W2 64-0331	43
W2 64-0332	43
W2 64-0333	43
W2 64-0334	43
W2 64-0335	43
W2 64-0336	60
W2 64-0339	87
W2 64-0340	60
W2 64-0341	43
W2 64-0342	43
W2 64-0343	43
W2 64-0347	45
W2 64-0348	45
W2 64-0349	46, 47, 115
W2 64-0350	114, 126
W2 64-0351	115, 116, 124
W2 64-0351	126
W2 64-0352	96, 101, 103
W2 64-0353	96, 101
W2 64-0354	104
W2 64-0355	104
W2 64-0356	104
W2 64-0357	59, 124, 125
W2 64-0358	59
W2 64-0359	32, 59
W2 64-0360	59, 119
W2 64-0361	59
W2 64-0362	22
W2 64-0363	46
W2 64-0364	46
W2 64-0365	47
W2 64-0366	47
W2 64-0367	49
W2 64-0368	49
W2 64-0369	49
W2 64-0370	50
W2 64-0371	50
W2 64-0372	51
W2 64-0373	51
W2 64-0374	51
W2 64-0375	46, 47, 49-51, 124
W2 64-0376	60
W2 64-0377	43
W2 64-0377	53
W2 64-0378	46, 47, 70
W2 64-0379	43
W2 64-0379	53
W2 64-0380	43
W2 64-0380	53
W2 64-0381	27
W2 64-0382	90
W2 64-0383	90
W2 64-0384	46, 49, 50, 65
W2 64-0385	79, 83
W2 64-0386	60
W2 64-0387	49
W2 64-0388	46, 47, 116
W2 64-0389	60
W2 64-0400	137, 141
W2 64-0401	137
W2 64-0401	141
W2 64-0402	137
W2 64-0403	137
W2 64-0404	137
W2 64-0405	137
W2 64-0406	137
W2 64-0407	137
W2 64-0408	137
W2 64-0409	137
W2 64-0410	137
W2 64-0411	137
W2 64-0412	137
W2 64-0413	137
W2 64-0414	137
W2 64-0415	137
W2 64-0416	137
W2 64-0417	137
W2 64-0418	137
W2 64-0419	137
W2 64-0420	137
W2 64-0421	137
W2 64-0422	146
W2 64-0423	137, 142
W2 64-0424	142
W2 64-0424	137
W2 64-0425	142
W2 64-0425	137
W2 64-0426	142
W2 64-0426	137
W2 64-0427	142
W2 64-0427	137
W2 64-0428	142
W2 64-0428	137
W2 64-0429	142
W2 64-0429	137
W2 64-0431	143
W2 64-0432	139
W2 64-0436	137
W2 64-0450	137
W2 64-0450	147
W2 64-0451	137
W2 64-0451	147
W2 64-0453	137
W2 64-0453	147
W2 64-0500	189
W2 64-0501	189
W2 64-0502	189
W2 64-0503	189
W2 64-0504	189
W2 64-0505	189
W2 64-0506	189
W2 64-0507	189
W2 64-0508	189
W2 64-0509	189
W2 64-0510	189
W2 64-0511	189
W2 64-0520	189
W2 64-0521	189
W2 64-0522	189
W2 64-0523	189
W2 64-0524	189
W2 64-0525	189
W2 64-0532	189
W2 64-0533	189
W2 64-0534	189
W2 64-0535	189
W2 64-0536	189
W2 64-0537	189
W2 64-0538	189
W2 64-0539	189
W2 64-0540	189
W2 64-0541	189
W2 64-0542	189
W2 64-0543	116
W2 64-0543	189
W2 64-0544	189
W2 64-0545	189
W2 64-0546	189
W2 64-0547	189
W2 64-0548	189
W2 64-0549	189
W2 64-0550	189
W2 64-0551	189
W2 64-0552	189
W2 64-0553	189, 191
W2 64-0554	189, 191
W2 64-0555	189, 191

Ordering Number Index

Order #	Page No.
W2 64-0556	189
W2 64-0557	189
W2 64-0558	189
W2 64-0559	189
W2 64-0560	189
W2 64-0561	189
W2 64-0562	189
W2 64-0563	189
W2 64-0564	102, 189
W2 64-0565	191
W2 64-0567	189
W2 64-0568	191
W2 64-0569	191
W2 64-0570	191
W2 64-0571	191
W2 64-0572	191
W2 64-0573	191
W2 64-0574	191
W2 64-0575	191
W2 64-0576	191
W2 64-0577	191
W2 64-0578	191
W2 64-0579	191
W2 64-0580	191
W2 64-0581	191
W2 64-0582	191
W2 64-0583	191
W2 64-0584	191
W2 64-0585	191
W2 64-0586	191
W2 64-0587	191
W2 64-0588	191
W2 64-0589	191
W2 64-0590	191
W2 64-0591	191
W2 64-0592	191
W2 64-0593	191
W2 64-0594	191
W2 64-0595	191
W2 64-0596	191
W2 64-0597	191
W2 64-0598	191
W2 64-0599	191
W2 64-0600	191
W2 64-0601	191
W2 64-0602	191
W2 64-0603	191
W2 64-0605	53
W2 64-0606	53
W2 64-0607	53
W2 64-0608	53
W2 64-0609	53
W2 64-0610	53
W2 64-0611	53
W2 64-0612	53
W2 64-0613	53
W2 64-0614	53
W2 64-0615	53
W2 64-0700	65
W2 64-0701	65
W2 64-0702	28, 49, 65
W2 64-0703	19, 28, 46, 49, 65
W2 64-0704	20, 26, 65
W2 64-0705	20-23, 49-51, 53, 65, 123
W2 64-0706	43, 65
W2 64-0707	25-27, 29, 31, 32, 43, 53, 65
W2 64-0708	18, 33, 65
W2 64-0709	34, 36-40, 65
W2 64-0710	35, 65
W2 64-0712	49, 65
W2 64-0713	49, 65
W2 64-0714	49, 50, 65
W2 64-0715	49-51, 65
W2 64-0716	65
W2 64-0717	65
W2 64-0744	235
W2 64-0745	234
W2 64-0746	236
W2 64-0749	235
W2 64-0750	70, 81, 86
W2 64-0751	70
W2 64-0752	70, 79, 81, 85, 86, 103
W2 64-0753	70, 79, 85
W2 64-0754	50, 53, 70, 79, 86
W2 64-0755	12, 13, 18-23, 25-34, 36-40, 50, 51, 53, 70, 79, 84, 86, 102, 103, 106
W2 64-0756	70, 79, 84
W2 64-0757	126
W2 64-0758	46, 47, 126
W2 64-0759	126
W2 64-0760	54, 125, 126
W2 64-0761	126
W2 64-0762	46, 47, 126
W2 64-0763	126
W2 64-0764	126
W2 64-0765	214
W2 64-0766	214
W2 64-0767	214
W2 64-0768	214
W2 64-0769	214
W2 64-0770	214
W2 64-0771	214
W2 64-0772	214
W2 64-0773	214
W2 64-0774	214
W2 64-0775	214
W2 64-0776	214
W2 64-0777	214
W2 64-0778	214
W2 64-0779	214
W2 64-0780	214
W2 64-0781	214
W2 64-0782	214
W2 64-0783	214
W2 64-0784	214
W2 64-0785	214
W2 64-0786	214
W2 64-0787	214
W2 64-0788	214
W2 64-0789	214
W2 64-0790	214
W2 64-0791	214
W2 64-0792	214
W2 64-0793	214
W2 64-0794	214
W2 64-0795	214
W2 64-0796	214
W2 64-0797	214
W2 64-0798	215
W2 64-0799	215
W2 64-0800	215
W2 64-0801	215
W2 64-0802	215
W2 64-0803	215
W2 64-0804	215
W2 64-0805	215
W2 64-0806	215
W2 64-0807	215
W2 64-0808	215
W2 64-0809	215
W2 64-0810	215
W2 64-0811	81, 215
W2 64-0812	216
W2 64-0813	216
W2 64-0814	216
W2 64-0815	216
W2 64-0816	216
W2 64-0817	216
W2 64-0818	216
W2 64-0819	216
W2 64-0820	216
W2 64-0821	133, 135
W2 64-0821	234
W2 64-0822	133, 135
W2 64-0822	234
W2 64-0823	133, 135
W2 64-0823	234
W2 64-0824	133, 135
W2 64-0824	234
W2 64-0825	236
W2 64-0826	236
W2 64-0827	236
W2 64-0828	236
W2 64-0837	235
W2 64-0838	235
W2 64-0839	235
W2 64-0840	235
W2 64-0841	234
W2 64-0842	234
W2 64-0843	234
W2 64-0844	234
W2 64-0845	236
W2 64-0846	236
W2 64-0847	236
W2 64-0848	236
W2 64-0857	235
W2 64-0858	235
W2 64-0859	235
W2 64-0860	235
W2 64-0861	234
W2 64-0862	234
W2 64-0863	234
W2 64-0864	234
W2 64-0865	237
W2 64-0866	237
W2 64-0867	237
W2 64-0868	237
W2 64-0877	235
W2 64-0878	235
W2 64-0879	235
W2 64-0880	235
W2 64-0900	230
W2 64-0901	230
W2 64-0902	230
W2 64-0903	230
W2 64-0904	230
W2 64-0905	230
W2 64-0906	230
W2 64-0907	230
W2 64-0908	230
W2 64-0909	230
W2 64-0910	230
W2 64-0911	230
W2 64-0912	230
W2 64-0913	230
W2 64-0914	230
W2 64-0915	230
W2 64-0916	230
W2 64-0917	230
W2 64-0918	230
W2 64-0919	230
W2 64-0920	230
W2 64-0921	230
W2 64-0922	230
W2 64-0923	230
W2 64-0924	230
W2 64-0925	230
W2 64-0926	230
W2 64-0927	230
W2 64-0928	230
W2 64-0929	230
W2 64-0930	230
W2 64-0931	230
W2 64-0932	231
W2 64-0933	231
W2 64-0934	231
W2 64-0935	231
W2 64-0936	231
W2 64-0937	231
W2 64-0938	231
W2 64-0939	231
W2 64-0940	231
W2 64-0941	231
W2 64-0942	231
W2 64-0943	231
W2 64-0944	231
W2 64-0945	231
W2 64-0946	231
W2 64-0947	231
W2 64-0948	231
W2 64-0949	231
W2 64-0950	231
W2 64-0951	231
W2 64-0952	231
W2 64-0953	231
W2 64-0954	231
W2 64-0955	231
W2 64-0956	231
W2 64-0957	231
W2 64-0958	231
W2 64-0959	231
W2 64-0960	231
W2 64-0961	231
W2 64-0962	231
W2 64-0963	231
W2 64-0964	157, 159
W2 64-0965	157, 159
W2 64-0966	157, 159
W2 64-0967	157, 159
W2 64-0968	234
W2 64-0969	236
W2 64-0972	235
W2 64-0973	234
W2 64-0974	237
W2 64-0977	235
W2 64-0978	133, 135
W2 64-0978	234
W2 64-0979	236
W2 64-0980	228
W2 64-0981	228
W2 64-0982	228
W2 64-0983	228
W2 64-0984	228
W2 64-0985	228
W2 64-0986	228
W2 64-0987	228
W2 64-0992	228
W2 64-0993	228
W2 64-0994	228
W2 64-0995	228
W2 64-0996	228
W2 64-0997	228
W2 64-0998	228
W2 64-0999	229
W2 64-1000	229
W2 64-1001	229
W2 64-1002	229
W2 64-1003	229
W2 64-1004	229
W2 64-1005	229
W2 64-1006	229
W2 64-1007	153
W2 64-1007	229
W2 64-1008	153
W2 64-1008	229
W2 64-1009	153
W2 64-1009	229
W2 64-1010	153
W2 64-1010	229
W2 64-1011	228
W2 64-1012	228
W2 64-1013	228
W2 64-1014	228
W2 64-1015	228
W2 64-1016	228

Ordering Number Index

Order #	Page No.
W2 64-1017	228
W2 64-1018	228
W2 64-1019	232
W2 64-1020	232
W2 64-1021	232
W2 64-1022	232
W2 64-1023	232
W2 64-1024	232
W2 64-1025	232
W2 64-1026	232
W2 64-1035	232
W2 64-1036	232
W2 64-1037	232
W2 64-1038	232
W2 64-1039	232
W2 64-1040	232
W2 64-1041	232
W2 64-1042	232
W2 64-1051	153
W2 64-1051	232
W2 64-1052	153
W2 64-1052	232
W2 64-1053	232
W2 64-1054	153
W2 64-1054	232
W2 64-1055	234
W2 64-1056	234
W2 64-1057	234
W2 64-1058	234
W2 64-1059	236
W2 64-1060	236
W2 64-1061	236
W2 64-1062	236
W2 64-1071	235
W2 64-1072	235
W2 64-1073	235
W2 64-1074	235
W2 64-1075	234
W2 64-1076	234
W2 64-1077	234
W2 64-1078	234
W2 64-1079	237
W2 64-1080	237
W2 64-1081	237
W2 64-1082	237
W2 64-1091	235
W2 64-1092	235
W2 64-1093	235
W2 64-1094	235
W2 64-1097	235
W2 64-1098	234
W2 64-1099	236
W2 64-1102	235
W2 64-1103	234
W2 64-1104	237
W2 64-1105	234
W2 64-1106	234
W2 64-1107	234
W2 64-1108	234
W2 64-1109	236
W2 64-1110	236
W2 64-1111	236
W2 64-1112	236
W2 64-1121	235
W2 64-1122	235
W2 64-1123	235
W2 64-1124	235
W2 64-1144	240
W2 64-1145	240
W2 64-1146	240
W2 64-1147	240
W2 64-1148	240
W2 64-1149	240
W2 64-1150	240
W2 64-1151	240
W2 64-1160	240
W2 64-1161	240
W2 64-1162	240
W2 64-1163	240
W2 64-1164	242
W2 64-1165	242
W2 64-1168	242
W2 64-1169	242
W2 64-1172	242
W2 64-1173	242
W2 64-1176	242
W2 64-1177	242
W2 64-1180	238
W2 64-1181	238
W2 64-1182	238
W2 64-1183	238
W2 64-1184	239
W2 64-1185	239
W2 64-1186	239
W2 64-1187	239
W2 64-1188	239
W2 64-1189	239
W2 64-1190	239
W2 64-1191	239
W2 64-1192	239
W2 64-1193	239
W2 64-1194	239
W2 64-1195	239
W2 64-1196	239
W2 64-1197	239
W2 64-1198	239
W2 64-1199	239
W2 64-1220	238
W2 64-1221	238
W2 64-1222	238
W2 64-1223	238
W2 64-1224	238
W2 64-1225	238
W2 64-1226	238
W2 64-1227	238
W2 64-1228	238
W2 64-1229	238
W2 64-1230	238
W2 64-1231	238
W2 64-1232	238
W2 64-1233	238
W2 64-1234	238
W2 64-1235	238
W2 64-1236	238
W2 64-1237	238
W2 64-1238	238
W2 64-1239	238
W2 64-1260	228
W2 64-1261	241
W2 64-1262	241
W2 64-1263	241
W2 64-1264	241
W2 64-1265	241
W2 64-1266	241
W2 64-1267	241
W2 64-1268	241
W2 64-1269	241
W2 64-1270	241
W2 64-1271	241
W2 64-1272	241
W2 64-1273	241
W2 64-1274	241
W2 64-1275	241
W2 64-1276	241
W2 64-1278	241
W2 64-1279	241
W2 64-1280	241
W2 64-1281	241
W2 64-1282	243
W2 64-1283	243
W2 64-1284	243
W2 64-1285	243
W2 64-1286	243
W2 64-1287	243
W2 64-1288	243
W2 64-1289	243
W2 64-1290	243
W2 64-1291	243
W2 64-1292	243
W2 64-1293	243
W2 64-1294	243
W2 64-1295	243
W2 64-1296	243
W2 64-1297	243
W2 64-1298	243
W2 64-1299	243
W2 64-1300	243
W2 64-1301	294
W2 64-1302	294
W2 64-1303	294
W2 64-1304	293
W2 64-1305	293
W2 64-1306	293
W2 64-1307	293
W2 64-1308	293
W2 64-1309	293
W2 64-1310	293
W2 64-1311	294
W2 64-1312	294
W2 64-1313	293
W2 64-1314	294
W2 64-1315	294
W2 64-1316	294
W2 64-1317	293
W2 64-1318	295
W2 64-1319	295
W2 64-1320	295
W2 64-1321	295
W2 64-1322	295
W2 64-1323	69, 161, 295
W2 64-1324	295
W2 64-1325	295
W2 64-1326	295
W2 64-1327	295
W2 64-1328	295
W2 64-1351	234
W2 64-1352	234
W2 64-1353	234
W2 64-1354	234
W2 64-1355	234
W2 64-1356	234
W2 64-1357	237
W2 64-1358	237
W2 64-1359	237
W2 64-1360	237
W2 64-1361	237
W2 64-1362	237
W2 64-1363	235
W2 64-1364	235
W2 64-1365	235
W2 64-1366	235
W2 64-1367	235
W2 64-1368	235
W2 64-1369	240
W2 64-1371	240
W2 64-1373	240
W2 64-1374	243
W2 64-1375	243
W2 64-1400	68
W2 64-1401	68
W2 64-1402	68
W2 64-1403	68, 124, 125
W2 64-1404	68, 124
W2 64-1405	68
W2 64-1406	32, 68
W2 64-1407	68
W2 64-1408	68
W2 64-1409	68
W2 64-1410	68
W2 64-1411	66
W2 64-1412	66
W2 64-1413	66
W2 64-1414	66
W2 64-1415	66
W2 64-1416	66
W2 64-1417	66
W2 64-1418	66
W2 64-1419	66
W2 64-1420	66
W2 64-1421	66
W2 64-1422	161
W2 64-1423	161
W2 64-1424	47, 51, 210
W2 64-1425	47, 51, 110, 210
W2 64-1426	69
W2 64-1427	96
W2 64-1428	69, 79
W2 64-1429	58, 70
W2 64-1430	96, 103
W2 64-1431	68
W2 64-1450	36
W2 64-1451	34
W2 64-1452	37
W2 64-1453	95
W2 64-1454	95
W2 64-1455	126
W2 64-1456	43
W2 64-1456	53
W2 64-1457	60
W2 64-1458	258
W2 64-1459-36	258
W2 64-1459-48	258
W2 64-1459-60	258
W2 64-1459-72	258
W2 64-1460	258
W2 64-1461-10	258
W2 64-1461-12	258
W2 64-1461-14	258
W2 64-1462	258
W2 64-1463	258
W2 64-1464	43
W2 64-1464WA	43
W2 64-1465M	105
W2 64-1466M	105
W2 64-1467M	105
W2 64-1468M	105
W2 64-1469M	105
W2 64-1470M	105
W2 64-1471M	105
W2 64-1472M	105
W2 64-1473M	105
W2 64-1474M	105
W2 64-1475M	105
W2 64-1476M	105
W2 64-1477M	105
W2 64-1478M	105
W2 64-1479M	105
W2 64-1480M	105
W2 64-1481	44
W2 64-1482	44
W2 64-1483	44
W2 64-1484	44
W2 64-1485	44
W2 64-1486	18
W2 64-1487	18
W2 64-1488	18
W2 64-1489	79, 86
W2 64-1490	79, 86
W2 64-1499	43, 65
W2 64-1500	43, 65, 126
W2 64-1503	100
W2 64-1506	58
W2 64-1507	58, 126
W2 64-1515	81
W2 64-1516	81
W2 64-1517	81
W2 64-1518	81
W2 64-1519	82
W2 64-1520	91
W2 64-1522	91, 92
W2 64-1523	78, 91, 92

Ordering Number Index

Order #	Page No.
W2 64-1526	18, 25-27, 29, 31, 33, 57
W2 64-1527	34, 37-39, 57
W2 64-1528	36, 40, 57
W2 64-1529	35, 57
W2 64-1530	57
W2 64-1531	32, 57
W2 64-1532	35
W2 64-1532	35
W2 64-1533	67
W2 64-1534	32
W2 64-1535	54
W2 64-1536	54
W2 64-1537	54
W2 64-1538	54
W2 64-1539	54
W2 64-1540	54
W2 64-1541	54
W2 64-1542	54, 125
W2 64-1543	126
W2 64-1543	115
W2 64-1544	126
W2 64-1545	98, 105, 109
W2 64-1545E	98, 105, 109
W2 64-1546	92
W2 64-1548	35
W2 64-1550	35, 67
W2 64-1551	35, 67
W2 64-1552	69
W2 64-1553	69
W2 64-1554	69
W2 64-1555	110
W2 64-1556	110
W2 64-1557	110
W2 64-1558	110
W2 64-1559	43
W2 64-1560	109
W2 64-1561	20-23, 57
W2 64-1562	28, 57
W2 64-1563	28, 57
W2 64-1564	19, 57
W2 64-1565	86
W2 64-1566	86
W2 64-1567	86
W2 64-1568	86
W2 64-1569	86
W2 64-1570	86
W2 64-1571	86
W2 64-1572	86
W2 64-1573	86
W2 64-1574	86
W2 64-1575	86
W2 64-1576	86
W2 64-1577	86
W2 64-1578	86
W2 64-1579	86
W2 64-1580	86
W2 64-1581	86
W2 64-1582	86
W2 64-1583	86
W2 64-1584	109
W2 64-1585	109
W2 64-1586	12, 13, 156
W2 64-1587	85
W2 64-1588	85
W2 64-1589	91
W2 64-1589	92
W2 64-1590	82
W2 64-1590E	82
W2 64-1591	129
W2 64-1592	119
W2 64-1593	105
W2 64-1594	105
W2 64-1600	308
W2 64-1601	308
W2 64-1602	308
W2 64-1603	308
W2 64-1605	201
W2 64-1606	98, 109
W2 64-1607	258
W2 64-1608	299
W2 64-1610	226
W2 64-1611	226
W2 64-1612	226
W2 64-1613	226
W2 64-1614	226
W2 64-1615	226
W2 64-1616	226
W2 64-1617	226
W2 64-177LE	82
W2 65-0001	301
W2 65-0002	299, 301
W2 65-0003	301
W2 65-0004	302
W2 65-0005	302
W2 65-0006	303
W2 65-0007	303
W2 65-0008	303
W2 65-0009	303
W2 65-0010	303
W2 65-0011	303
W2 65-0012	303
W2 65-0013	303
W2 65-0014	303
W2 65-0015	303
W2 65-0016	97, 123
W2 65-0017	303
W2 65-0018	303
W2 65-0019	303
W2 65-0020	303
W2 65-0021	303
W2 65-0022	303
W2 65-0023	303
W2 65-0029	303
W2 65-0030	303
W2 65-0040	121
W2 65-0041	122
W2 65-0043	117
W2 65-0044	118
W2 65-0045	97, 120-122, 129
W2 65-0047	121-123
W2 65-0049	117
W2 65-0050	117
W2 65-0051	117
W2 65-0052	118, 120-123
W2 65-0053	118, 123
W2 65-0054	123
W2 65-0055	123
W2 65-0056	97, 123
W2 65-0057	97, 123, 129
W2 65-0058	123
W2 65-0059	123
W2 65-0060	123
W2 65-0061	123
W2 65-0062	123
W2 65-0063	123
W2 65-0064	121-123
W2 65-0065	121-123
W2 65-0066	123
W2 65-0067	123
W2 65-0070	123
W2 65-0071	121-123
W2 65-0072	121-123
W2 65-0073	127, 129
W2 65-0074	128, 129
W2 65-0075	128, 129
W2 65-0076	127, 129
W2 65-0076	315
W2 65-0078	129
W2 65-0079	129
W2 65-0080	129
W2 65-0081	129
W2 65-0082	129
W2 65-0083	129
W2 65-0084	129
W2 65-0086	129
W2 65-0087	129
W2 65-0088	127, 129
W2 65-0090	129
W2 65-0091	129
W2 65-0093	123
W2 65-0098	97, 123, 129
W2 65-0100	121, 122, 129
W2 65-0101	120
W2 65-0103	120
W2 65-0104	129
W2 65-0105	89
W2 65-0109	118
W2 65-0207	220
W2 65-0208	220
W2 65-0219	165
W2 65-0220	168
W2 65-0221	169
W2 65-0222	167
W2 65-0223	167
W2 65-0224	168
W2 65-0225	170
W2 65-0227	171
W2 65-0229	172
W2 65-0230	172
W2 65-0231	172
W2 65-0236	172
W2 65-0237	173
W2 65-0239	173
W2 65-0240	173
W2 65-0241	173
W2 65-0242	173
W2 65-0243	174
W2 65-0244	175
W2 65-0247	175
W2 65-0252	176
W2 65-0253	179
W2 65-0254	180
W2 65-0255	180
W2 65-0256	181
W2 65-0259	181
W2 65-0260	183
W2 65-0261	183
W2 65-0266	184
W2 65-0276	184
W2 65-0283	164
W2 65-0283S	164
W2 65-0284	186
W2 65-0285	186
W2 65-0286	186
W2 65-0287	186
W2 65-0288	186
W2 65-0289	186
W2 65-0290	186
W2 65-0291	186
W2 65-0292	186
W2 65-0293	186
W2 65-0294	186
W2 65-0295	186
W2 65-0296	186
W2 65-0297	186
W2 65-0298	186
W2 65-0299	186
W2 65-0300	186
W2 65-0301	186
W2 65-0302	186
W2 65-0303	186
W2 65-0304	186
W2 65-0305	186
W2 65-0306	186
W2 65-0307	186
W2 65-0308	186
W2 65-0309	186
W2 65-0310	186
W2 65-0311	186
W2 65-0312	186
W2 65-0313	186
W2 65-0314	186
W2 65-0319	186
W2 65-0320	186
W2 65-0321	186
W2 65-0322	186
W2 65-0323	172
W2 65-0323	186
W2 65-0363	184, 186
W2 65-0325	186
W2 65-0329	211
W2 65-0337	211
W2 65-0337	212
W2 65-0385	186
W2 65-0386	186
W2 65-0387	186
W2 65-0388	186
W2 65-0389	169
W2 65-0390	169
W2 65-0391	169
W2 65-0392	169
W2 65-0393	169
W2 65-0394	169
W2 65-0395	169
W2 65-0396	168
W2 65-0550	211
W2 65-0608	127
W2 65-0630	176, 177
W2 65-0631	171
W2 65-0632	186
W2 65-0633	186
W2 65-0634	186
W2 65-0635	186
W2 65-0636	186
W2 65-0637	186
W2 65-0638	169
W2 65-0641	212
W2 65-0642	169
W2 65-0643	174
W2 65-1525	129
W2 66-0001	193
W2 66-0002	193
W2 66-0003	193
W2 66-0004	193
W2 66-0005	196
W2 66-0006	195
W2 66-0007	195
W2 66-0008	194
W2 66-0009	193, 195
W2 66-0010	193, 195
W2 66-0012	193, 195
W2 66-0013	194
W2 66-0014	194
W2 66-0015	194
W2 66-0016	196
W2 66-0017	196
W2 66-0018	195
W2 66-0019	195
W2 66-0020	195
W2 66-0021	195
W2 66-0022	196
W2 66-0023	195, 196
W2 66-0024	195, 196
W2 66-0025	195, 207
W2 66-0026	194
W2 66-0027	194
W2 66-0028	193
W2 66-0029	193
W2 66-0032	194
W2 66-0033	193
W2 66-0034	194
W2 66-0035	193
W2 66-0036	194
W2 66-0037	193
W2 66-0038	194
W2 66-0039	193
W2 66-0040	194
W2 66-0041	193
W2 66-0042	194
W2 66-0043	193

Ordering Number Index

Order #	Page No.
W2 66-0046	194
W2 66-0047	193
W2 66-0048	193, 195
W2 66-0049	195
W2 66-0050	195
W2 66-0053	196
W2 66-0054	196
W2 66-0055	196
W2 66-0056	196
W2 66-0057	195, 196
W2 66-0058	196
W2 69-0006	265
W2 69-0007	265
W2 69-0008	265
W2 69-0009	265
W2 69-0010	265
W2 69-0011	265
W2 69-0012	265
W2 69-0013	264, 265
W2 69-0014	264, 265
W2 69-0016	264, 265
W2 69-0020	287
W2 69-0021	287
W2 69-0022	287
W2 69-0023	290
W2 69-0024	290
W2 69-0025	290
W2 69-0026	267
W2 69-0027	267
W2 69-0028	267
W2 69-0029	264
W2 69-0037	265
W2 69-0038	265
W2 69-0048	265
W2 69-0049	265
W2 69-0050	265
W2 69-0051	265
W2 69-0052	265
W2 69-0053	290
W2 69-0054	266
W2 69-0055	266
W2 69-0070	288
W2 69-0071	288
W2 69-0072	288
W2 69-0073	288
W2 69-0074	288
W2 69-0075	288
W2 69-0076	288
W2 69-0077	288
W2 69-0078	288
W2 69-0079	288
W2 69-0080	288
W2 69-0081	288
W2 69-0082	288
W2 69-0092	289
W2 69-0105	310
W2 69-0107	310
W2 69-0112	99
W2 69-0114	220
W2 69-0117	99
W2 69-0120	244, 246
W2 69-0130	307
W2 69-0131	307
W2 69-0132	307
W2 69-0133	307
W2 69-0134	307
W2 69-0135	307
W2 69-0136	307
W2 69-0137	307
W2 69-0138	307
W2 69-0139	307
W2 69-0140	307
W2 69-0141	307
W2 69-0142	307
W2 69-0150	223
W2 69-0151	223
W2 69-0152	305
W2 69-0153	305
W2 69-0154	305
W2 69-0155	305
W2 69-0156	305
W2 69-0157	305
W2 69-0158	305
W2 69-0160	305
W2 69-0161	223
W2 69-0162	223
W2 69-0163	305
W2 69-0164	305
W2 69-0165	305
W2 69-0166	305
W2 69-0167	305
W2 69-0225	256
W2 69-0226	256
W2 69-0227	256
W2 69-0229	256
W2 69-0230	256
W2 69-0231	256
W2 69-0232	256
W2 69-0233	256
W2 69-0234	256
W2 69-0235	256
W2 69-0236	256
W2 69-0237	256
W2 69-0250	315
W2 69-0251	315
W2 69-0252	315
W2 69-0253	315
W2 69-0254	315
W2 69-0255	315
W2 69-0256	315
W2 69-0257	315
W2 69-0258	315
W2 69-0259	315
W2 69-0260	315
W2 69-0262	315
W2 69-0300	208
W2 69-0301	208
W2 69-0302	208
W2 69-0303	208
W2 69-0316	220
W2 69-0317	220
W2 69-0318	220
W2 69-0350	312
W2 69-0351	312
W2 69-0353	312
W2 69-0354	312
W2 69-0368	313
W2 69-0369	313
W2 69-0370	313
W2 69-0371	313
W2 69-0372	313
W2 69-0373	313
W2 69-0376	313
W2 69-0377	313
W2 69-0378	313
W2 69-0379	313
W2 69-0380	313
W2 69-0381	313
W2 69-0382	313
W2 69-0383	313
W2 69-0384	225
W2 69-0385	225
W2 69-0387	225
W2 69-0388	225
W2 69-0389	225
W2 69-0390	225
W2 69-0391	225
W2 69-0392	225
W2 69-0394	225
W2 69-0395	225
W2 69-0438	225
W2 69-0440	313
W2 69-0442	312
W2 69-0443	312
W2 69-0444	312
W2 69-0445	312
W2 69-0446	312
W2 69-0447	312
W2 69-0448	225
W2 69-0452	271
W2 69-0453	271
W2 69-0454	271
W2 69-0455	271
W2 69-0456	271
W2 69-0457	271
W2 69-0458	271
W2 69-0459	271
W2 69-0463	271
W2 69-0464	271
W2 69-0465	271
W2 69-0476	271
W2 69-0477	271
W2 69-0479	271
W2 69-0490	284, 290
W2 69-0491	284
W2 69-0492	285
W2 69-0493	285
W2 69-0494	89, 284
W2 69-0495	286
W2 69-0496	286
W2 69-0497	286
W2 69-0499	284
W2 69-0502	269
W2 69-0503	269
W2 69-0504	269
W2 69-0505	269
W2 69-0506	269
W2 69-0507	269
W2 69-0508	269
W2 69-0509	269
W2 69-0510	269
W2 69-0511	269
W2 69-0867	303
W2 69-0868	303
W2 69-0869	303
W2 69-0930	199
W2 69-0931	199
W2 69-0932	209
W2 69-0933	202
W2 69-0934	202
W2 69-0935	202
W2 69-0936	203
W2 69-0937	203
W2 69-0938	203
W2 69-0939	203
W2 69-0940	203
W2 69-0941	203
W2 69-0942	203
W2 69-0943	203
W2 69-0944	203
W2 69-0945	203
W2 69-0946	203
W2 69-0947	203
W2 69-0950	209
W2 69-0951	209
W2 69-0952	209
W2 69-0955	205
W2 69-0956	205
W2 69-0957	205
W2 69-0958	205
W2 69-0959	205
W2 69-0960	205
W2 69-0961	205
W2 69-0962	205
W2 69-0963	205
W2 69-0964	205
W2 69-0965	205
W2 69-0966	205
W2 69-0968	205
W2 69-0969	205
W2 69-0970	205
W2 69-0971	205
W2 69-0972	205
W2 69-0973	205
W2 69-0974	205
W2 69-0975	205
W2 69-0976	205
W2 69-0987	205
W2 69-0988	205
W2 69-0989	205
W2 69-0990	205
W2 69-0991	205
W2 69-0992	205
W2 69-0993	205
W2 69-0997	205
W2 69-0998	205
W2 69-1003	203
W2 69-1005	203
W2 69-1010	316
W2 69-1011	316
W2 69-1012	316
W2 69-1013	316
W2 69-1014	316
W2 69-1015	316
W2 69-1016	316
W2 69-1017	316
W2 69-1060	296
W2 69-1061	296
W2 69-1062	296
W2 69-1064	296
W2 69-1065	296
W2 69-1066	248, 251-253, 256
W2 69-1067	248, 251-253, 256
W2 69-3000	278
W2 69-3001	278
W2 69-3006	280
W2 69-3007	280
W2 69-3008	280
W2 69-3009	280
W2 69-3010	280
W2 69-3011	280
W2 69-3012	280
W2 69-3013	280
W2 69-3016	282
W2 69-3018	282
W2 69-3019	282
W2 69-3021	281
W2 69-3023	283
W2 69-3024	283
W2 69-3027	282
W2 69-3028	282
W2 69-3032	282
W2 69-3033	280
W2 69-3050	265
W2 69-3051	265
W2 69-3052	265
W2 69-3053	265
W2 69-3054	265
W2 69-3055	265
W2 69-3056	265
W2 69-3057	265
W2 69-3058	265
W2 69-3059	265
W2 69-3060	265
W2 69-3061	265
W2 69-3100	318
W2 69-3101	317
W2 69-3102	317
W2 69-3103	317
W2 69-3104	317
W2 69-3105	317
W2 69-3106	317
W2 69-3107	317
W2 69-3108	317
W2 69-3109	318
W2 69-3110	318
W2 69-3111	317
W2 69-3130	155
W2 69-3140	245, 247
W2 69-3145	206
W2 70-2027	74

Ordering Number Index

Order #	Page No.
W2 70-2116	89
W2 70-2217	73
W2 70-2222	72
W2 70-2223	72
W2 72-0001	75
W2 72-0002	75
W2 72-0008	75
W2 72-0215	320
W2 72-0216	320
W2 72-0217	320
W2 72-0218	320
W2 72-0219	321
W2 72-0220	321
W2 72-0221	321
W2 72-0222	321
W2 72-0223	321
W2 72-0224	321
W2 72-0226	322
W2 72-0227	319, 322
W2 72-0231	320
W2 72-0232	320
W2 72-0233	324
W2 72-0234	320
W2 72-0235	320
W2 72-0236	321
W2 72-0237	321
W2 72-0238	323
W2 72-0239	323
W2 72-0240	323
W2 72-0242	326
W2 72-0245	325
W2 72-0246	325
W2 72-0247	325
W2 72-0248	324
W2 72-0249	322
W2 72-0250	322
W2 72-0251	322
W2 72-0252	322
W2 72-0257	322
W2 72-0258	322
W2 72-0262	326
W2 72-0264	326
W2 72-0265	326
W2 72-0266	327
W2 72-0267	327
W2 72-0268	327
W2 72-0269	327
W2 72-0270	329
W2 72-0271	329
W2 72-0272	329
W2 72-0273	329
W2 72-0274	329
W2 72-0275	329
W2 72-0276	329
W2 72-0277	329
W2 72-0278	329
W2 72-0279	329
W2 72-0280	329
W2 72-0283	328
W2 72-0284	328
W2 72-0285	328
W2 72-0286	328
W2 72-0287	328
W2 72-0288	328
W2 72-0289	328
W2 72-0290	328
W2 72-0291	328
W2 72-0292	328
W2 72-0293	328
W2 72-0294	328
W2 72-0295	328
W2 72-0296	328
W2 72-0297	328
W2 72-0298	328
W2 72-0299	328
W2 72-0300	328
W2 72-0301	328
W2 72-0302	328
W2 72-0304	327
W2 72-0305	322
W2 72-0308	328
W2 72-0313	328
W2 72-0314	328
W2 72-0315	328
W2 72-0316	328
W2 72-0317	328
W2 72-0318	328
W2 72-0323	329
W2 72-0324	329
W2 72-0325	329
W2 72-0326	329
W2 72-0328	329
W2 72-0329	328
W2 72-0330	328
W2 72-0331	328
W2 72-0332	328
W2 72-0333	328
W2 72-0334	328
W2 72-0335	328
W2 72-0336	328
W2 72-0337	330
W2 72-0339	330
W2 72-0340	330
W2 72-0341	330
W2 72-0342	330
W2 72-0343	330
W2 72-0344	330
W2 72-0348	322
W2 72-0349	322
W2 72-0350	322
W2 72-0351	322
W2 72-0352	322
W2 72-0353	322
W2 72-0354	322
W2 72-0356	322
W2 72-0460	265
W2 72-1015	89
W2 72-1920	265, 267
W2 72-1922	265, 267
W2 72-1972	265, 267
W2 72-2987	277
W2 72-4220	178
W2 72-4221	182
W2 72-4222	171
W2 72-4223	171
W2 72-4224	171
W2 72-4656	323
W2 72-4657	323
W2 72-4658	323
W2 72-4659	323
W2 72-4660	323
W2 72-4661	323
W2 72-4662	323
W2 72-4666	317, 322
W2 72-4701	259
W2 72-4702	259
W2 72-4703	259
W2 72-4704	259
W2 72-4706	259
W2 72-4707	259
W2 72-4708	259
W2 72-4709	259
W2 72-4711	259
W2 72-4712	259
W2 72-4713	259
W2 72-4714	259
W2 72-4716	259
W2 72-4717	259
W2 72-4719	259
W2 72-4720	259
W2 72-4721	259
W2 72-4722	259
W2 72-4724	259
W2 72-4725	259
W2 72-4726	259
W2 72-4727	259
W2 72-4728	257
W2 72-4729	257
W2 72-4730	257
W2 72-4731	257
W2 72-4732	257
W2 72-4733	257
W2 72-4734	257
W2 72-4735	257
W2 72-4736	257
W2 72-4737	259
W2 72-4738	259
W2 72-4739	259
W2 72-4740	259
W2 72-4741	260
W2 72-4742	260
W2 72-4743	260
W2 72-4744	260
W2 72-4745	260
W2 72-4746	260
W2 72-4747	260
W2 72-4748	260
W2 72-4749	260
W2 72-4750	260
W2 72-4751	260
W2 72-4752	260
W2 72-4753	260
W2 72-4754	260
W2 72-4755	257
W2 72-4756	257
W2 72-6021	259
W2 72-6023	259
W2 72-6030	244, 249
W2 72-6031	244, 249
W2 72-6032	244, 249
W2 72-6033	249
W2 72-6034	249
W2 72-6051	249
W2 72-6180	269
W2 72-6181	269
W2 72-6186	280
W2 72-6187	280
W2 72-6188	280
W2 72-6194	320
W2 72-6195	319
W2 72-6196	319
W2 72-6197	319
W2 72-6198	319
W2 72-6475	306
W2 72-6476	306
W2 72-6477	306
W2 72-6478	306
W2 72-6479	306
W2 72-6480	306
W2 72-6481	306
W2 72-6482	306
W2 72-6486	309
W2 72-6487	309
W2 72-6488	309
W2 72-6489	309
W2 72-6490	309
W2 72-6491	309
W2 72-6492	309
W2 72-6493	309
W2 72-6494	309
W2 72-6495	309
W2 72-6496	309
W2 72-6497	309
W2 72-6498	309
W2 72-6499	309
W2 72-6500	309
W2 72-6501	309
W2 72-6502	309
W2 72-6503	309
W2 72-6504	309
W2 72-6505	309
W2 72-6506	309
W2 72-6507	309
W2 72-6508	309
W2 72-6509	309
W2 72-6510	309
W2 72-6511	309
W2 72-6512	309
W2 72-6513	309
W2 72-6514	309
W2 72-6515	309
W2 72-7141	289
W2 72-7582	309
W2 72-7583	309
W2 72-7584	309
W2 72-7585	309
W2 72-7586	309
W2 72-7587	309
W2 72-7588	309
W2 72-7589	309
W2 72-7590	309
W2 72-7591	309
W2 72-7592	309
W2 72-7593	309
W2 72-7594	309
W2 72-7595	309
W2 72-7596	309
W2 72-7597	309
W2 72-7598	309
W2 72-7599	309
W2 72-7600	309
W2 72-7601	309
W2 72-7602	309
W2 72-7603	309
W2 72-7604	309
W2 72-7605	309
W2 72-7606	309
W2 72-7607	309
W2 72-7608	309
W2 72-7609	309
W2 72-7610	309
W2 72-7611	309
W2 72-7733	259
W2 72-7734	259
W2 73-0000	254
W2 73-0001	254
W2 73-0003	245, 255
W2 73-0004	291
W2 73-0005	291
W2 73-0006	291
W2 73-0007	291
W2 73-0008	292
W2 73-0009	292
W2 73-0011	245, 255
W2 73-0117	277
W2 73-0118	277
W2 73-0119	277
W2 73-0120	277
W2 73-0122	277
W2 73-0124	277
W2 73-0210	277
W2 73-1523	277
W2 7507-023	195
W2 7507-028	195

Product Index

3-Channel, Difference Amplifier, NL143 174
4-Channel Conditioner, NL530 181
35 mm Dish Format
- Closed Bath Chambers 46, 48, 50
- Culture Dish Chamber 45, 46, 47
- Culture Dish Inserts 44
- Disposable Inserts 44
- Field Stimulation Chambers 47
- for QE-1 & DH Series 48-51, 65
- High Profile Chambers 50
- Low Profile Chambers 49
- Open Bath Chambers 44, 45, 47-51

50 mm Dish Format
- Dish Inserts 54
- Chamber Inserts, Disposable 54

A

AC Preamplifier, NL104A 168
AC Signal Delay, NL202 175
AC-DC Amplifier, NL106 170
Accessories
- for Chambers 65-70
- for Culture Dish Heaters 126
- for Fiber Optic Systems 326, 327, 329
- for PDMI-2, PSMI, CSMI & Leiden Chambers 123
- for Platforms 58, 59
- for Superfusion Systems 129
- for Syringe Holder Systems 86
- for Temperature Control Systems 110, 111
- for Tissue Sectioning Systems 313
- for Valve Control Systems 79, 86
- for Warner Micro-incubation Chambers 126

Acquisition Hardware & Software 150
Agar Bridge Reference Electrode Kit.....69
Aluminosilicate Capillary Glass 219
Amplifiers
- AC-DC, Neurolog™, NL106 170
- Audio, Neurolog™, NL120S 172
- Bilayer Clamp 138, 139
- Difference, 3-Channel, NL143 174
- Pressure, Neurolog™, NL108A 171
- 2-Channel Voltage/Current Clamp System 202
- Bessel Filter with DC Differential Amplifier 162
- Bilayer Clamp 138
- Computer Controlled 206
- Differential Amplifier 160, 161
- EasyMount, Harvard & NaviCyte 198
- Intracellular Electrometers 157, 158
- Low Pass Filters with Gains 163
- Multi-Channel Voltage/Current Clamp Systems 203
- Oocyte Clamp 152
- Patch Clamp 132, 134
- Single Channel Epithelial Voltage Clamps 200
- Single Channel Voltage/Current Clamp for Epithelial Tissues 199
- Stimulus Isolation Unit – Bipolar 209

Audio Amplifier, NL120S 172, 180
Auto Chloridizer Kit, 863 291
Automatic Oscillating Tissue Slicer 314, 315

B

Backlights, Glass Fiber 330
Base, Bright/Darkfield 330
Bases, Magnetic 256
BenchMate Platforms 259
Bilayer Workstation
- Introduction 136
- Bilayer Clamp Amplifier 138, 139
- Bilayer Perfusion System 143
- BLM Starter Kit 146
- Classic Bilayer Chambers & Cuvettes 141
- Faraday Cages 140
- Headstage Holder Kit 146
- Instrument Rack 146
- Lamp, Stirplate & Dual Function Controller 144
- Low-Pass Bessel Filter 143
- Perfusion Bilayer Chamber 142

Bilayer Workstation Accessories
- 50 MHz Dual Channel Oscilloscope 149
- Acquisition Hardware & Software 150
- Channel Simulator - Fixed Model 148
- Channel Simulator - Variable Model 148
- Dual Dipole Stirrer 144
- Glass Capillary Tubing 149
- Low Temperature Halogen Lamp 144
- On-Site Setup & Training 147
- Planar Lipid Bilayer Thermocycler 147
- Power Line Conditioning 149
- Stereo Zoom Microscope 149
- Stirbars 149

Biphasic Pulse Buffer, NL512 182
Bipolar Temperature Controller 96, 97
Blank Module NL50, Neurolog™ 165
Books.....296
Borosilicate Capillary Glass 214-219
- Capillary Glass with Filament 218
- Double Barrel Special 218
- Glass Rod 219
- Multi-Barrel 219
- Premium Capillary Glass 214-215
- Standard Wall without Filament 217
- Theta Glass 218
- Thin Wall without Filament 217

Brain/Tissue Slice Chamber System 127-129
Bright/Darkfield, Base 330
Buffers
- Biphasic Pulse, Neurolog™, NL512 182
- DURACAL™ pH 289
- Pulse, Neurolog™, NL510 181
- Redox 289

C

Cages, Faraday 140
Calibration Module, NL410 176
Capillary Glass
- Clark Capillary Glass 217, 218, 219
- Glass Capillary Tubing for Bilayer 149
- Patch Clamp Glass 216
- Pipette Sterilization 220
- Premium Capillary Glass 214, 215

Cell Injectors
- 8- and 4-Channel Pressure Injection Systems 304, 305
- Auto Nanoliter Injector 307
- Chemical Drilling Micropipettes 309
- Harvard/Medical Pico-Injector Systems 300-302
- Pico Injection/Micromanipulator System 299
- PLI-100 & PLI-90 300-302
- Screw-Actuated Syringes 310
- SLAM Soft Lipid-Assisted Microinjection Micropipettes 308
- ZonaDrill™ Laser System 306

Chambers, Electrode, Neurolog™, NL101 169
Chamber (Imaging & Recording)
- Accepts Slice Anchors 18, 24, 29, 31, 33-37, 40
- Accessories 65-70
- Closed Bath 19, 20, 21, 41, 46, 50
- Confocal Imaging 41, 52
- Disposable 32, 44, 54
- Field Stimulation 21, 38, 47, 51
- for 35 mm culture dishes 44-47
- for 50 mm culture dishes 54
- Inserts 44-47, 54
- Large Volume (>300 ul) 14, 20, 34-38, 40, 49, 50, 54
- Low Profile 31, 49, 51
- Oocyte 12-14, 33
- Patch 14, 18, 29, 31, 32, 37-39
- Quick Change with Coverslip Bottom 48-51
- Rectangular Bath 34-38, 40
- Silicone 32
- Sloped inflow 18, 35
- Slotted Bath 12, 13, 21, 39, 41, 44, 47, 51
- Small Volume (< 100 ul) 12, 13, 19, 26-28, 41, 44, 49, 51, 54

Product Index

- Tissue Slice Recording 23, 24, 29, 32, 34-38, 40
- Transepithelial 52
- Ultra-quiet 18, 35
- Upright Microscope Compatible 14, 18, 22-24, 27, 29, 31-38, 40, 41
- with Slice Support 35, 36, 40

Chamber Accessories
- Agar Bridge Reference Electrode Kit 69
- Coverslips 65
- Mini Magnetic Clamps 69
- Nylon Mesh Kit 67
- PE(Polyethylene)Tubing 70
- Silicone Grease Kit 70
- Slice Anchor Kits 67
- Slice Anchor Supports 67
- Slice Anchors 66
- Slice Support with Nylon Grid 67
- Suction & Perfusion Tubes 68
- Suction Tube Upgrade Kit for Series 20 Chambers 20, 70

Chambers, Classic Bilayer .....141 - 142

Chamber Systems
- Brain/Tissue Slice Chamber System 127-129
- Classic Ussing System 187, 188
- Navicyte Diffusion & Ussing Systems 192-197

Channel Stimulator
- Fixed Model 148
- Variable Model 148

Clamps
- Computer Controlled Current & Voltage Clamp with Software 206
- Multi-Channel Voltage/Current Clamp Systems 203
- Voltage/Current Clamps 198-200

Clark Capillary Glass
- Aluminosilicate Capillaries with Filament 219
- Borosilicate Double Barrel Special 218
- Borosilicate Glass Rod 219
- Borosilicate Multi-Barrel 219
- Borosilicate Standard Wall without Filament 217
- Borosilicate Theta Glass 218
- Borosilicate Thin Wall without Filament 217
- Borosilicate with Filament 218

Classic Bilayer Chambers & Cuvettes ..141

Closed Bath Chambers
- Closed Bath Chamber Insert 46
- Confocal Imaging Chamber 41
- for QE-1 & DH Series 50
- for Transepithelial Studies 52
- Large Closed Diamond Bath 20
- Slotted Bath for Field Stimulation 21
- Small Volume Closed Bath Imaging Chambers 19

CO_2
- Harvard CO_2 Gas/pH Controller 89
- Micro-CO_2 Electrode 284

Cold Light Sources
- Intralux 5100 319
- Intralux DC 1100 & Filters 321
- IWL-500e 320
- Spare Lamps & Power Cords 322
- V-Lux 1000 320

Computer Controlled Current & Voltage Clamp with Software 206

Confocal Imaging Chamber
- Imaging Chambers for Transepithelial Studies 52
- Low Profile, Closed Bath, Customizable 41 - 43

Conditioner, 4-Channel, Neurolog™, NL530 181

Constant Current, Stimulus, Isolator, NL800A.....184

Continuous Flow Tubing Segments 75

Controllers
- Gas Controllers 89, 90
- Microdrive Controller 864 254
- Perfusion Valve Controllers 76, 78
- Temperature Controllers 94, 96-98, 108
- Dual Function Controller for Bilayer Workstation 144

Control Units for Motorized Micromanipulators
- 3-Direction Joystick Control Unit 251
- Push Button Control Unit 251

Cooled Inserted Stage 99

Cooled Platforms
- CSMI Microscope Stage Microincubator 120
- PDMI-2 Open Perfusion Micro-incubator 117
- PSMI Patch Slice Micro-incubator 118

Corning Type 7740 (Pyrex) 214

Counter, Neurolog™, NL603 183

Cover Glasses 65

Culture Dish Heaters
- 35 mm Format 114-116, 124
- 50 mm Format 125
- Accessories 126

Culture Dishes (35 & 50 mm).....126

Cuvettes, Classic Bilayer Chambers 141

D

Data Acquistion
- Acquisition Hardware & Software for Bilayer 150
- HAI 118 Iworks Data Acquistion System for Oocytes 154, 155
- Respirometry Software 279

DC Pre-Amplifier, NL102G 166

De Fonbrune Microforge 224, 225

Delay Width NL405 177

Difference Amplifier, 3-Channel, NL143 174

Diffusion
- Horizontal Diffusion Chamber System 196
- Vertical Diffusion/Ussing Chambers 204
- Vertical & Horizontal System 195
- Vertical Ussing & Horizontal Diffusion Chamber System 192
- Vertical Ussing/Diffusion Chambers 194

Dishes, Glass Bottom Cell Culture.....126

Disposable, Chambers
- 35 mm Chamber Inserts 44
- 50 mm Chamber Inserts 54
- Silicone Imaging Chamber 32

Disposable, Pressure Transducer, NL108T2 172

Dissolved Oxygen Measurement & Respirometry Systems
- 1-2 Channel Oxygen Meter 278
- 6 Electrode Respirometer 281
- Flow Cell, FC 100 283
- General Electrode Holder, EH 100 283
- Microcathode Oxygen Electrode 280
- MicroCell Model, MC 100 282
- Mitocell Miniature Respirometer 280
- 6-Channel Oxygen System, Model 928 278
- Respiration Cells, RC 300 & RC 350 282
- Respirometry Software 279

Dissolved Oxygen Meter & Electrodes
- 2 mm Oxygen Electrode 267
- Dissolved Oxygen Meter 267

Dummy Membranes 208

DURACAL™ pH & Redox Buffers 289

E

8-Pole Low-Pass Bessel Filter 143

Easy Mount Chamber System.....204 - 205

Electrodes
- AMANI 'LEAK FREE' Microcombination pH Electrodes 287
- Buffer, DURACAL™ pH & Redox Buffers 289
- Combination Gastroesophageal pH Electrode 286
- Combination pH Electrode for Micro Wells 284
- Combination pH Electrode in 11 Gauge SS Tube 286
- Combination pH Electrode in 20 Gauge Needle 285
- Combination pH Electrode in 18 Gauge SS Tube 285
- Flexible Combination pH Electrode for Free Flap Surgery 286
- Leak-Free Reference Electrodes 290
- Protein Resistant pH Electrodes 288
- Single pH Electrode in 25 Gauge Needle 284

Warner Instruments Inc. • Phone (203) 776-0664 • Toll Free U.S. (800) 599-4203 • Fax (203) 776-1278 • **www.warneronline.com**

Product Index

Electrode Chambers, NL101 169

Electrode Holders

- Electrode Holder Replacement Parts 243
- Electrode/Manifold Holder Holders 242
- Holder for Theta Glass 242
- PE Series for Microperfusion 240
- ME Series for Electrocal & Pressure Applications 238, 239
- Micro, Tungsten, Neurolog™, NL04 169
- MP Series for Microinjection 241
- E Series Intracellular Recording & Microiontophoresis 227-232
- Q Series for Patch Clamp (Warner & Axon) 233-237

EMG Integrator, NL703 184

Epithelial

- Epithelial Transport: A Guide to Methods & Experimental Analysis 296
- Chamber for Epithelial Applications 52
- Single Channel Epithelial Voltage Clamps 200
- Single Channel Voltage/Current Clamp for Epithelial Tissues 199
- Excised Patch Chamber 39

Ergo/Olympus SZ/SD Ringlight.....326

F

4-Point Standard Ringlight 324

Faraday Cages 140

Fast Exchange Open Diamond Bath 26, 27

Fast-Step Perfusion Systems

- Standard System 80-82
- System with Mini-Valves 82

Fiber Optic

- Backlights & Base 330
- Light Guides 327, 328
- Light Guides Accessories 329
- Light Sources 319-321
- Light Source Accessories 322
- Ringlights 323-325
- Ringlights Accessories 326

Fiber Optic Light Guides

- Articulating Arm with Heavy Steel Base 329
- Flexible Light Guides 328
- Gooseneck Accessories 327
- Gooseneck Light Guides 327
- Incident Gooseneck Light Guides 328
- Modular Accessory System 329

Fiber Optic Oxygen Sensing System 270

Fiber Optic Ringlights

- 4-Point Standard Ringlight 324
- Accessories for Standard/Compact Ringlights 326
- Compact Ringlight 324
- Ergo/Olympus SZ/SD Ringlight 326
- Mini Ringlight 325
- Ringlight Adapters 322
- SMD/MAXI Ringlight 325
- Standard Ringlight 323
- White LED Ringlights 323

Field Stimulation, Chambers....21, 38, 47, 51

Filters

- 8-Pole Bessel Filter with DC Differential Amplifier LPF-8 162
- High Pass, Neurolog™, NL144 173
- Low Pass Filters LPF-100B & LPF-202A 163
- Neurolog™ System, For 173

Flat Nitric Oxide Sensor 263

Flip-Flop, NL505.....180

Flexible Light Guides 327, 328

Flow Control

- Electrode/Manifold Holders 88
- Manifolds & Flow Control Hardware 87
- Syringe Needles 86
- Tubing & Connector Kit 86
- Vacuum/Solution Flow Valves 88

FO_2ton Fiber Optic Oxygen Sensing Sytem 270

G

Gas Bubbler Manifolds 85

Gas Controllers

- CO_2 Gas/pH Controller 89
- Dual Stream O_2 & CO_2 Controller 90

Gate, Logic, Neurolog™, NL501 179

Generator

- Period, Neurolog™, NL304 176
- Pulse, Neurolog™, NL301 175
- Pulse, Neurolog™, NL412 178

Glass

- Glass Fiber Backlights 330
- Cell Culture Dishes, Glass Bottom 126

Glass, Capillary

- Aluminosilicate 219
- Borosilicate, Capillary Glass with Filament 218
- Borosilicate, Double Barrel Special 218
- Borosilicate, Glass Rod 219
- Borosilicate, Multi-Barrel 219
- Borosilicate, Premium Capillary Glass 214-215
- Borosilicate, Standard Wall without Filament 217
- Borosilicate, Theta Glass 218
- Borosilicate, Thin Wall without Filament 217
- Clark Capillary Glass 217, 218, 219
- Patch Clamp Glass 216
- Pipette Sterilization 220
- Premium Capillary Glass 214, 215

Glass Coverslips 65

Gooseneck

- Light Guides 327, 328
- Light Guide Accessories 329

Grease Kit, Silicone 70

H

Haas Top for Brain/Tissue Slice Chamber 128

HAI 118 Data Acquistion System 154, 155

Harvard CO_2 Gas/pH Controller 89

Harvard Apparatus / Medical Systems

- Alignment Rings 123
- CSMI Microscope Stage Microincubator 120
- Chambers 119
- Fixing Platforms 123
- Leiden Closed Perfusion Micro-Incubator 122
- Leiden Open Micro-Incubator 121
- Micro-Incubator Accessories 123
- Microscope Stage Incubators 120 - 123
- Patch Slice Micro-Incubators 118
- PLI-100 Pico-Injector 300
- PLI-90 Pico-Injector 302
- Open Perfusion Micro-Incubator PDMI-2 117

Heated Platforms

- 35 mm dish format 124
- 50 mm dish format 125
- CSMI Microscope Stage Incubator 120
- DH-35 Culture Dish Heater 114
- Heated Platform for Chambered Slides & 1 x 3 Slides 119
- Leiden Closed 122
- Leiden Open 121
- PDMI-2 Open Perfusion Micro-Incubator 117
- PSMI Patch Slice Micro-Incubator 118

Heated Top Coverslip for DH-35i & DH-40i Chambers.....126

Heater/Cooler Jackets for Series 20 Chambers 104

High Pass Filter, NL144.....173

Halogen

- Fiber Optic Cold Light Sources 320, 321
- High Intensity Cold Halogen Light Source 319
- Lamp for Bilayer, Low Temperature 144

Holders

- Electrode Holder Replacement Parts 243
- Electrode/Manifold Holders 242
- Holder for Theta Glass 242
- PE Series for Microperfusion 240
- ME Series for Electrocal & Pressure Applications 238, 239
- Micro, Tungsten, Neurolog™, NL04 169
- MP Series for Microinjection 241

Product Index

E Series Intracellular Recording & Microiontophoresis 227-232
Q Series for Patch Clamp (Warner & Axon) 233-237

Horizontal
Diffusion Chamber System 196
Vertical & Horizontal System 195
Vertical Ussing & Horizontal Diffusion Chamber System 192

I

Iontophoresis
E Series Electrode Holders 227-232
Micropipette, 7 Barrel 220

Illumination
Backlights & Base 330
Fiber Optic Cold Light Sources 320, 321
Fiber Optic Ringlights 323-325
Gooseneck Light Guides 327, 328
High Intensity Cold Halogen Light Source 319
Light Guide Accessories 329
Light Source Spare Parts & Accessories 322
Ringlights & Accessories 323 - 326

Imaging & Recording Chambers
Confocal Imaging Chambers 41
Coverslip Insertion Option 29
Excised Patch Chamber 39
Fast Exchange Open Diamond Bath 26, 27
Large Bath Chamber with Slice Supports 36
Large Closed Diamond Bath 20
Large Rectangular Open Bath Chamber 34
Narrow Bath Chamber with Field Stimulation 38
Narrow Rectangular Bath Chamber 37
Oocyte 12-14, 33
Open Diamond Bath 22, 24, 26, 27
Open Diamond Bath with Low Profile 31
Open Round Bath 23
RC Series 14
Round Coverslip Chambers 28
Silicone Imaging Chamber 32
Slotted Bath for Field Stimulation 21
Small Volume Closed Bath 19
Ultra-quiet 18, 35
Very Large Rectangular Open Bath Chamber for Slice Studies with Atmospherics 40

In-line Solution Temperature Control
Dual In-line Solution Heater/Cooler 101
Eight Line Heater 103
Fast Flow Heater 100
Heater/Cooler Jackets for Series 20 Chambers 104
Multi-Line Heaters 102
Slow Flow Heater 100

Infusion Pumps
Peristaltic 74, 75
Syringe 72, 73

Injectors
8- and 4-Channel Pressure Injection Systems 304, 305
Nanoject II Auto Nanoliter Injector 307
Chemical Drilling Micropipettes 309
Harvard/Medical Pico-Injector Systems 300-302
Pico Injection/Micromanipulator System 299
PLI-100 & PLI-90 300-302
Screw-Actuated Syringes 310
SLAM Soft Lipid-Assisted Microinjection Micropipettes 308
ZonaDrill™ Laser System 306

inNO-T Nitric Oxide Measurement System 262-265
Input Manifolds 208

Inserted Stages
Cooled Inserted Stages 99
Warmed Inserted Stages 99

Inserts, Chamber
35 mm 44-47
50 mm 54
Disposable 44, 54
Field Stimulation 47, 51
Perfusion 45-47

Instrument Rack for Bilayer Workstation 146

Integrator
EMG, Neurolog™, NL703 184
Pulse, Neurolog™, NL601 183

Interface Cables 58
Intracellular Electrometers 157, 158

Intralux Fiber Optic Illuminators
Model 5100 319
Model DC 1100 321

Inverted Microscope 318
Isolation, Bipolar Stimulus Isolation Unit 209

Isolation, Vibration
BenchMate Platforms 259
VIBRALITE Breadboards 260
VIBRAPLANE Workstations 257, 258

Isolator-Constant Current, Stimulus, NL800A 184

J

Joystick Control Unit for Micromanipulator 251
Joystick Micromanipulator 252

K

Kits
Agar Bridge Reference Electrode Kit 69
Auto Chloridizer Kit 291
Bilayer Workstation Starter Kit 146
Headstage Holder Kit 146
Nylon Mesh Kit 67
Magnetic Clamp Kit 59
Microelectrode Starter Kit 292
Series 20 Chambers Kit 59
Silicone Grease Kit 70
Slice Anchor Kits 67
Suction Tube Upgrade Kit for Series 20 Chambers 20, 70
Tubing & Connector Kit 86

L

Lamps
Fiber Optic 319 - 330
for Bilayer Workstation 144

Large Volume Chambers
Chamber Inserts, 50mm, RC-61T-05 & RC-61T-06 54
Confocal Imaging Chamber, RC-30 41 - 43
Confocal Imaging Chamber, RC-30HV 41 - 43
Confocal Imaging Chamber, RC-30WA 41 - 43
Large Bath Chamber with Slice Supports, RC-27L 36
Large Closed Diamond Bath, RC-21 20
Large Closed Diamond Bath, RC-21BR 20
Narrow Rectangular Bath Chamber with Field Stimulation, RC-27NE 38
Narrow Rectangular Bath Chamber, RC-27N 37
Quick Change, High Profile Chamber, RC-40HP 50
Quick Change, Low Profile Chamber, RC-40LP 49
Recording Chambers, RC-10 14
Recording Chambers, RC-11 14
Recording Chambers, RC-13 14
Recording Chambers, RC-16 14
Rectangular Open Bath Chamber, RC-27 34
Ultra-Quiet Imaging Chamber for Slice Studies, RC-27D 35
Ultra-Quiet Imaging Chamber for Slice Studies, RC-27LD 35
Very Large Rectangular Open Bath with Atmospherics, RC-29 40

LED Ringlights, White Light 323

Leiden Micro-Incubators
Micro-Incubator, LU-CB1 121
Closed Perfusion Chamber, LU-CPC-CEH 122

Light Guides
Accessories 329

Warner Instruments Inc. • Phone (203) 776-0664 • Toll Free U.S. (800) 599-4203 • Fax (203) 776-1278 • **www.warneronline.com**

Product Index

Flexible Fiber Optic 327, 328

Light Sources

Fiber Optic Cold Light Sources 320, 321
High Intensity Cold Halogen Light Source 319
Lamp for Bilayer, Low Temperature 144

Logic Gate, Neurolog™, NL501.....179

Low Pass Filters

8-Pole Low-Pass Bessel Filter 143
8-Pole Bessel Filter with DC Differential Amplifier 162
Low Pass Filters LPF-100B & LPF-202A 163
Neurolog™ System, For, NL134, NL135, NL136 173

Low Temperature Halogen Lamp for Bilayer.....144

Lubricant, Silicone Grease Kit 70

M

Magnetic Bases 256

Magnetic Clamps

Kit for Series 20 Chambers 59
Mini Magnetic Clamps 69

Manifolds

Flow Control Electrode/Manifold Holders 88
Gas Bubbler Manifolds 85
Holder for Electrode/Manifolds 242
Input Manifolds & Dummy Membranes 208
Manifolds & Flow Control Hardware 87

McIlwain Mechanical Tissue Chopper 316

Medical Systems/Harvard Appartus

Alignment Rings 123
CSMI Microscope Stage Microincubator 120
Chambers 119
Fixing Platforms 123
Leiden Closed Perfusion Micro-Incubator 122
Leiden Open Micro-Incubator 121
Micro-Incubator Accessories 123
Microscope Stage Incubators 120 - 123
Patch Slice Micro-Incubators 118
PLI-100 Pico-Injector 300
PLI-90 Pico-Injector 302
Open Perfusion Micro-Incubator PDMI-2 117

Membranes, Dummy.....208

Metal Electrodes

Ag-AgCl Electrodes 293, 294, 295
Auto Chloridizer Kit 291
Microelectrode Starter Kit 292
Reference Cells 293

Micro-Electrode Holder, Tungsten, NL04 169

Micro-Incubation Chambers

Very Large Rectangular Open Bath, Series 20 40

Micro-Incubation Systems

Accessories 123
CSMI 120
DH-35i 115
DH-40i 116
Leiden Closed 122
Leiden Open 121
PDMI-2 117
PSMI 118

Microdrive

Controller 254
Microdrive 864/1 255
Microdrive 864/2 255

Microelectrode

Holders 232 - 243
Pullers 222, 226
Microforges, De Fonbrune 224
Microforge-Grinding Center 226
Starter Kit for Microelectrodes 292

Microforge

De Fonbrune Microforge 224, 225
Microforge-Grinding Center 226

Micro-Incubators.....114 - 123

Microinjection

Auto Nanoliter Injector 307
Chemical Drilling Micropipettes 309
Harvard/Medical Pico-Injector Systems 300-302
Multi-Channel Pressure Injection Systems 304, 305
Pico Injection/Micromanipulator System 299
Screw-Actuated Syringes 310
SLAM Soft Lipid-Assisted Microinjection Micropipettes 308
ZonaDrill™ Laser System 306

Micromanipulators

Control Units for Motorized Manipulators 251
Dovetail Slide 249
General Purpose 246
Integra 247
Joystick Control 252
Selection Guide 244, 245
Standard Manual Control 248
Standard Motorized Control 250
Ultraprecise 253

Microminiature Electrodes

Amani Microcombination pH Electrodes 287
CO_2 Electrode 284
Combination pH Electrode 20 Ga Needle 285
Combination pH Electrode for Gastroesophageal 286
Combination pH Electrode for Micro Wells 284
Combination pH Electrode in 11 Ga Stainless Steel Tube 286
Combination pH Electrode in 18 Ga Stainless Steel Tube 285
Flexible pH Electrode for Flap Surgery 286
Flexible Reference Electrode 290
Leek-Free Reference Electrodes 290
Protein Resistant pH Electrodes 288
Single pH Electrode 25 Ga (no reference) 284

Micropipettes

Chemical Drilling Micropipettes 309
SLAM Soft Lipid-Assisted Microinjection Micropipettes 308

Microscopy

Inverted Microscope 318
Stereo Zoom Microscope 317

Mini Peristaltic Pumps 74, 75

Multi-Line Solution Heaters .....100 - 103

N

Nanoject II Auto Nanoliter Injector 307

Navicyte Diffusion & Ussing Systems 192-197

NeuroLog™ System

NL04 Tungsten Micro-Electrode Holder 169
NL100AK Headstage 168
NL100RK Pre-Amplifier & Stimulus Relay 169
NL101 Electrode Chambers 169
NL102G DC Pre-Amplifier 166
NL104A AC Preamplifier 168
NL106 AC-DC Amplifier 170
NL107 Transducer Amplifier 170
NL108A Pressure Amplifier 171
NL108T2 Disposable Pressure Transducer 172
NL108T4 Pressure Transducer 171
NL120S Audio Amplifier 172
NL125 & 126 Filters 173
NL134 Low Pass Filter 173
NL135 Low Pass Filter 173
NL136 Low Pass Filter 173
NL143 Three Channel Difference Amplifier 174
NL144 High Pass Filter 173
NL201 Spike Trigger 174
NL202 AC Signal Delay 175
NL301 Pulse Generator 175
NL304 Period Generator 176
NL405 Width Delay 177
NL410 Calibration Module 176
NL412 Pulse Generator 178
NL50 Blank Module 165
NL501 Logic Gate 179
NL505 Flip-Flop 180
NL506 Analog Switch 180
NL510 Pulse Buffer 181

Product Index

NL512 Biphasic Pulse Buffer 182
NL530 4-Channel Conditioner 181
NL601 Pulse Integrator 183
NL603 Counter 183
NL703 EMG Integrator 184
NL800A Stimulus Isolator-Constant Current 184
NL822 & NL824 Pre-Amplifiers 185
Rack (Case) with Power Supply 164

Nitrate Reductor 266

Nitric Oxide inNO-T Nitric Oxide Measurement System 262-265

Nitric Oxide Sensors
amiNO-100 Sensor 263
amiNO-2000 Sensor 263
amiNO-30 Sensor 263
amiNO-600 Sensor 263
amiNO-7 Sensor 263
amiNO-FLAT Sensor 264
amiNO-IV Sensor 264

Nylon Mesh Kit 67

O

Objective Warmers 105

Olympus/Ergo SZ/SD Ringlight 326

Oocyte
Clamp OC-725C for Oocyte 152, 153
HAI 118 Iworks Data Acquistion System for Oocytes 154, 155
Recording Chamber 12-14, 33
Steel Base Plate 13
Two-Electrode Voltage Clamp Work Station TEV700 156

Oscilloscope, 50 MHz Dual Channel 149

Oxygen
Dissolved Oxygen Measurement & Respirometry System 278-283
Dissolved Oxygen Meter & Electrodes 267
Dual Chamber Oxygen Measuring System 272, 273, 274
FO_2ton Fiber Optic Oxygen Sensing Sytem 270
Oxystat System for Oxygen Consumption Measurements 275, 276, 277
PMOD 2000 Phosphorescence O_2 Measurement System 268, 269
Respirometry Software 279

Oxygen Measuring System, Dual Chamber
Batch/Flow Chamber System 273
Dual-Channel Oxygen Amplifier 274
Electrode Chlorider 274
Oxygen Electrodes 273
Precision Stirring Controllers 274
Single Chamber Systems with Electrodes 274

Oxystat System, O_2 Consumption 275

P

Patch Clamp, Chambers ....14, 18, 29, ...31, 32, 37-39

Patch Clamp Glass
Corning 7056 Capillary Glass 216
Corning 8161 Capillary Glass 216
Custom 8520 Capillary Glass 216

PE (Polyethylene) Tubing 70

PDMI-2 Open Perfusion Micro-Incubator 117

Peltier
Controller 96, 97
In-line Solution Heater/Cooler 101
Open Perfusion Micro-incubator 117
Patch Slice Micro-incubator 118
Stage Insert 99

Perfusion Systems
Bilayer Perfusion System 143
Fast-Step 80-82
Fast-Step, Mini-valve 82

Peristaltic Pumps
Harvard Mini-Peristaltic Pump 74
Model 720 & Tube Sets 75

pH
AMANI 'LEAK FREE' Microcombination pH Electrodes 287
Buffer, DURACAL™ pH & Redox Buffers 289
Combination Gastroesophageal pH Electrode 286
Combination pH Electrode for Micro Wells 284
Combination pH Electrode in 11 Gauge SS Tube 286
Combination pH Electrode in 20 Gauge Needle 285
Combination pH Electrode in 18 Gauge SS Tube 285
DURACAL™ pH & Redox Buffers 289
Flexible Combination pH Electrode for Free Flap Surgery 286
Leak-Free Reference Electrodes 290
Protein Resistant pH Electrodes 288
Single pH Electrode in 25 Gauge Needle 284

PHC Series Heater/Cooler Jackets 104

Phosphorescence O_2 Measurement System 268

Pipette Holders ....227 - 243

Pipette Pullers
De Fonbrune Microforge 224, 225
Microforge-Grinding Center 226
Programmable Pipette Puller 222, 223

Pipette Storage Container 220

Planar Lipid Bilayer Workstation ....136 - 151

Platforms
Classic Series 20 55
PM Series (Magnetic, for Series 20) 56

Platforms, Accessories
Magnetic Clamp Kit 59
Platform & Chamber Parts 58
Series 20 Interface Cables 58
Thermistors 58

PLI-100 Pico-Injector 300

PLI-90 Pico-Injector 302

Potash Rubium Lead Capillary Glass 216

Power Line Conditioning for Bilayer 149

Power Supply with Rack (Case) 164

Pre-Amplifier
AC, Neurolog™, NL104A 168
& Stimulus Relay, NL100RK 169
DC, Neurolog™, NL102G 166
Neurolog™, NL822 & NL824 185

Prechamber for Brain/Tissue Slice System 127

Precision Dissolved Oxygen Measurement/Respirometry System ....278 - 283

Premium Capillary Glass
Standard Wall Borosilicate 214
Standard Wall Borosilicate with Filament 214
Theta Glass 215
Thin Wall Borosilicate 214
Thin Wall Borosilicate with Filament 215

Pressure
Amplifier, Neurolog™, NL108A 171
Transducer, Disposable, Neurlog, NL108T2 172

Programmable Pipette Puller 222, 223

Protein Resistant pH Electrodes 288

PSMI Patch Slice Micro-Incubator 118

Pullers
De Fonbrune Microforge 224, 225
Microforge-Grinding Center 226
Programmable Pipette Puller 222, 223

Pulse
Buffer, Biphasic, Neurolog™, NL512 182
Buffer, Neurolog™, NL510 181
Integrator, NL601 183
Generator, Neurolog™, NL301 175
Generator, Neurolog™, NL412 178

Pumps
Peristaltic 74, 75
Syringe 72, 73

Push Button Control Unit for Motorized Manipulators 251

Product Index

R

Racks
- Bilayer Instrument Rack 146
- Rack (Case) with Power Supply 164

RC Series
- Chambers 14
- Stage Adapters 15

Redox Buffers, DURACAL™ 289

Reference Electrodes
- Flexible Reference Electrode 290
- Leek-Free Reference Electrodes 290

Respirometers 278-283

Respirometry
- 1-2 Channel Oxygen Meter 278
- 6 Electrode Respirometer 281
- Flow Cell FC 100 283
- General Electrode Holder EH 100 283
- Microcathode Oxygen Electrode 280
- MicroCell Model MC 100 282
- Mitocell Miniature Respirometer 280
- Model 928, 6-Channel Oxygen System 278
- Respiration Cells RC 300 & RC 350 282
- Respirometry Software 279

Ringlights
- 4-Point Standard Ringlight 324
- Accessories for Standard/Compact Ringlights 326
- Compact Ringlight 324
- Ergo/Olympus SZ/SD Ringlight 326
- Mini Ringlight 325
- SMD/MAXI Ringlight 325
- Standard Ringlight 323
- White LED Ringlights 323

Round Coverslip Chambers 28

S

Screw-Actuated Air Syringes.....310

Screw-Actuated Micrometer Driven Hamilton Syringe 310

Sensors
- amiNO-100 Nitric Oxide Sensor 263
- amiNO-2000 Nitric Oxide Sensor 263
- amiNO-30 Nitric Oxide Sensor 263
- amiNO-600 Nitric Oxide Sensor 263
- amiNO-7 Nitric Oxide Sensor 263
- amiNO-FLAT Nitric Oxide Sensor 264
- amiNO-IV Nitric Oxide Sensor 264

Series 20 Chambers
- General Information 16
- Chamber Slotted Bath for Field Stimulation 21
- Chambers with Coverslip Insertion Option 29
- Excised Patch Chamber with Two Slotted Open Baths 39
- Fast Exchange Open Diamond Bath Chambers 26
- Large Bath Chamber with Slice Supports 36
- Large Closed Diamond Bath 20
- Large Rectangular Open Bath Chamber 34
- Narrow Bath Chamber with Field Stimulation 38
- Narrow Rectangular Bath Chamber 37
- Open Diamond Bath 22
- Open Diamond Bath for Fast Fluid Exchange 27
- Open Diamond Bath for Oocyte Studies 33
- Open Diamond Bath for Tissue Slice Studies 24
- Open Diamond Bath with Low Profile 31
- Open Round Bath 23
- Round Coverslip Chambers 28
- Silicone Imaging Chamber 32
- Small Volume Closed Bath Imaging Chambers 19
- Ultra-quiet Imaging Chamber for Biological Specimens 18
- Ultra-quiet Imaging Chamber for Slice Studies 35
- Very Large Rectangular Open Bath Chamber for Slice Studies with Atmospherics 40

Series 30 Chambers
- Cell Culture Dish Perfusion Chamber Insert 45, 46, 47
- Confocal Imaging Chambers, RC-30 41
- Disposable Perfusion Inserts for 35 mm Dishes 44

Series 40
- High Profile & Closed Bath Chambers 50
- Low Profile Chambers for 12, 15, 18 & 25 mm Coverslips 49
- Quick Change Coverslip Bottom Imaging Chambers 48
- Slotted Bath Low Profile Chambers 51

Series 50
- Imaging Chambers for Transepithelial Studies 52

Series 60
- 50 mm Disposable Chamber Inserts 54

Signal Delay, AC, Neurolog™ NL202..175

Silicone
- Grease Kit 70
- Imaging Chamber 32

Silver-Silver Chloride Electrodes 293

SLAM Soft Lipid-Assisted Microinjection Micropipettes 308

Slice Chamber with Atmospherics 40

Slicers for Tissue
- Automatic Oscillating Tissue Slicer 314, 315
- McIlwain Mechanical Tissue Chopper 316
- Vibratome® 311, 313

Slices
- Anchors for 66
- Supports for 67
- Ultra-Quiet Imaging Chamber for Slice Studies 35

Software
- Acquisition Hardware & Software for Bilayer 150
- Computer Controlled Current & Voltage Clamp with Software 206
- HAI 118 Iworks Data Acquistion System for Oocytes 154, 155
- Respirometry Software 279

Solution Temperature Control
- Dual In-line Solution Heater/Cooler 101
- Eight Line Heater 103
- Fast Flow Heater 100
- Heater/Cooler Jackets for Series 20 Chambers 104
- Multi-Line Heaters 102
- Slow Flow Heater 100

Specimen
- Deluxe Bath 313
- Mounting Blocks 313
- Mounts 1⁄2 inch Head 313
- Retriever 313
- Tray 313
- Ultra-quiet Imaging Chamber for Biological Specimens 18

Spike Trigger, NL201 174

Spill Control
- Overflow Sensor 91
- Spill Sensor 92

Stage Adapters
- RC Series 15
- Series 20 60
- Series 30 43

Starter Kit, Bilayer 146

Stereo Zoom Microscopes 149, 317

Stimulus Isolator-Constant Current, NL800A.....184

Stimulus Relay & Pre-Amplifier, NL100RK 169

Stirbars 149

Stirplate & Dual Function Controller 144

Stirrer Dual Dipole 144

Suction & Perfusion Tubes 68, 70

Superfusion.....127-129
- Accessories 129
- Base Unit 127
- Haas Top 128
- Temperature Controllers 129
- Zbicz Top 128

Switch, Analog, Neurolog™ NL506 180

Syringe Holder Systems
- Accessories 86
- Constant Flow 84

Product Index

- Gas Bubbler Manifold 85
- Modular & Fixed Series 83

Syringe Pump
- Low RFI Syringe Pump for Physiological Experiments 72
- Nanomite 73

Syringe Warmers
- 6 x 10 cc Syringe Package 106
- Modular Syringe Heating System 108
- Single 60 cc Syringe Package 107
- Syringe Pump Syringe Warmers 109

Syringe, Screw Actuated
- Screw-Actuated Air Syringes 310
- Screw-Actuated Micrometer Driven Hamilton Syringe 310

T

Tables
- BenchMate Platforms 259
- VIBRALITE Breadboards 260
- VIBRAPLANE Workstations 257, 258

Temperature Controller
- Battery Powered 98
- Bipolar 96, 97
- Computer Controllable 96
- Cooler 96, 97
- Dual Channel 94
- Heater 94, 96-98
- High Temperature 94
- Low Cost 98
- Single Channel 94, 96-98
- Syringe Heating System 108

Temperature Controller Accessories
- Cables & Thermistors 110
- Holders for In-line Solution Heaters 110
- Power Interface 111
- Syringe Heater Stand 111

Thermistors 58, 110

Thermocycler for Planar Lipid Bilayer 147

Theta Capillary Glass 218

Thin Wall Capillary Glass
- Clark with Filament 218
- Clark without Filament 217
- Premium with Filament 215
- Premium without Filament 214

Three Channel Difference Amplifier, NL143 174

Tissue Sectioning
- Automatic Oscillating Tissue Slicer 314, 315
- McIlwain Mechanical Tissue Chopper 316
- Vibratome® 311, 313

Tissue/Slice Chambers
- Chambers with Coverslip Insertion Option 29
- Large Bath Chamber with Slice Supports 36
- Large Rectangular Open Bath Chamber 34
- Narrow Bath Chamber with Field Stimulation 38
- Narrow Rectangular Bath Chamber 37
- Open Diamond Bath for Tissue Slice Studies 24
- Silicone Imaging Chamber 32
- Ultra-Quiet Imaging Chamber for Slice Studies 35
- Very Large Rectangular Open Bath Chamber for Slice Studies with Atmospherics 40

Training, On-Site for Bilayer Workstation 147

Transducer
- Amplifier, Neurolog™, NL107 170
- Disposable Pressure, Neurolog™, NL108T2 172
- Pressure, Neurolog™, NL108T4 171
- Transducer Amplifier 170

Trigger, Spike, Neurolog™, NL201 174

Tubing, Capillary Glass 149

Tungsten Micro-Electrode Holder, NL04 169

U

Ultraprecise Micromanipulator 253

Ussing
- 2-Channel Voltage/Current Clamp System 202
- Classic Ussing System 187, 188
- Computer Controlled Current & Voltage Clamp with Software 206
- Horizontal Diffusion Chamber System 196
- Input Manifolds & Dummy Membranes 208
- Multi-Channel Voltage/Current Clamp Systems 203
- Self-Contained Ussing Chambers 190
- Vertical & Horizontal System 195
- Vertical Diffusion/Ussing Chambers 204
- Vertical Ussing & Horizontal Diffusion Chamber System 192
- Vertical Ussing/Diffusion Chambers 194
- Voltage/Current Clamps 198-200

V

V-Lux 1000 Fiber Optic Illuminator 320

Valve Control Systems
- 6 Channel Systems 76
- 8 Channel Systems 78
- Parts & Accessories 79, 86
- Perfusion Fast-Step 80-82
- Perfusion Fast-Step, Mini-valve 82

Vertical Systems
- Diffusion/Ussing Chambers 204
- Vertical & Horizontal System 195
- Ussing & Horizontal Diffusion Chamber System 192
- Ussing/Diffusion Chambers 194

VIBRALITE Breadboards 260

VIBRAPLANE Workstations 257, 258

Vibration Isolation
- BenchMate Platforms 259
- VIBRALITE Breadboards 260
- VIBRAPLANE Workstations 257, 258

Vibratome®
- Deluxe Specimen Bath 313
- Glass Knife Adapter 313
- Sapphire Knife 313
- Section Mounting Device 313
- Specimen Mounting Blocks 313
- Specimen Mounts 1/2 inch Head 313
- Specimen Retriever 313
- Specimen Tray 313
- Tissue Sectioning System Accessories 313
- V-Block Adapter 313
- Vibratome® 1000 Classic 311
- Vibratome® 1000 Plus 311
- Vibratome® 1500 312
- Vibratome® 3000 Deluxe 311
- Vibratome® 3000 Plus 311
- Vibratome® Care Package 313
- Vibratome® The Works 313

Voltage/Current Clamps
- Computer Controlled Current & Voltage Clamp with Software 206
- Multi-Channel Voltage/Current Clamp Systems 203
- Single Channel Epithelial Voltage Clamps 200
- Single Channel Voltage/Current Clamp for Epithelial Tissues 199
- Voltage/Current Clamps 198-200

W

Warmed Inserted Stages 99

Width Delay, Neurolog™ System, NL405 177

White Light Illuminator 320

Z

Zbicz Top for Brain/Tissue Slice Chamber 128

ZonaDrill™ Laser System 306

Zoom Microscope, Stereo 317

Technical Support, Ordering, Payment, Delivery, Terms and Conditions

Technical Support & Domestic Orders*

Warner Instruments
1125 Dixwell Avenue
Hamden, CT 06514 USA

phone	**800.599.4203 (toll-free)** **203.776.0664**
fax	**203.776.1278**
e-mail	**support@warneronline.com**
website	**www.warneronline.com**

Domestic Orders*

Harvard Apparatus
84 October Hill Road
Holliston, MA 01746-1388 USA

phone	**800.272.2775 (toll-free)** **508.893.8999**
fax	**508.429.5732**
e-mail	**bioscience@harvardapparatus.com**
website	**www.harvardapparatus.com**

** See inside back cover for distributors outside of the United States.*

Payment Options

Purchase Order

Terms are net 30 for customers with pre-approved credit.

Credit Card

Visa, MasterCard, American Express and Discover are accepted.

Prepayment

To prepay, send check or money order with your purchase order. Call Harvard Apparatus customer service in advance for exact shipping charges or include your UPS or FedEx account number. All checks should be made payable to Harvard Apparatus, in U.S. Dollars and drawn on a U.S. bank.

Delivery Options

Shipping

Shipping charges are added to your invoice. Orders ship UPS Ground service unless otherwise requested. FOB Hamden, CT 06514

Terms and Conditions



Return Policy

If unsatisfied with a product purchased from Harvard Apparatus you may return the item for credit or replacement. You must contact us within thirty days of receipt of your shipment to obtain a Return Authorization Number and instructions to facilitate the return process. All returned products are subject to inspection and approval by Harvard Apparatus prior to issuing credit or replacement. Products must be in original manufacturer's packaging and include all instructions, manuals, and inserts. Products returned in new condition will be charged a 15% restocking fee or a minimum of $30.00. Products not in saleable condition will be returned to the customer or assessed a refurbishment fee.

Harvard Apparatus will provide full credit for the following:

1. **Items not supplied in accordance with your order.**
2. **Items that are defective at the time of receipt.**

Returns not acceptable for credit include:

1. **Items that have been customized**
2. **Items that are outdated, shelf-worn, damaged, or used and therefore unsuitable for return to stock for resale**
3. **Chemicals or sterile items that have been opened**
4. **Product(s) that have been exposed to harmful, toxic or hazardous substances**

Repairs

If your product is out of warranty but requires repair, you must contact Harvard Apparatus and obtain a Return Authorization Number and instructions to facilitate the return process. All repairs are subject to the following:

1. **Repair orders charged on a time and materials basis**
2. **$150 per hour for labor with a $150 minimum labor charge**
3. **All repairs are performed on a first in/first out basis, only after receipt of a valid purchase order**
4. **Estimates available upon request**
5. **Some older products may not be repairable due to component obsolescence**

Minimum Orders

We appreciate all orders and therefore have no minimum order requirement, however, a small handling fee of $10 will be added to orders below $75.

Sales Subsidiaries & Authorized Dealers

Subsidiaries

CANADA

Harvard Apparatus Canada
Attn: Sales Department
6010 Vanden Abeele
Saint-Laurent, Quebec H4S 1R9
Canada

phone **514.335.0792 • 800.361.1905** (canada only)
fax **514.335.3482**
e-mail **sales@harvardapparatus.ca**
website **www.harvardapparatus.ca**

FRANCE

Harvard Apparatus, S.A.R.L.
Attn: Sales Department
6 Avenue des Andes
Miniparc – Bat. 8
91952 Les Ulis Cedex, France

phone **33.1.64.46.00.85**
Fax **33.1.64.46.94.38**
e-mail **info@harvardapparatus.fr**
website **www.harvardapparatus.fr**

GERMANY

Hugo Sachs Elektronik
Harvard Apparatus, GmbH
Gruenstrasse 1
D-79232 March-Hugstetten, Germany

phone **49.7665.92000**
fax **49.7665.920090**
e-mail **info@hugo-sachs.de**
website **www.hugo-sachs.de**

UNITED KINGDOM

Harvard Apparatus, Ltd.
Attn: Sales Department
Fircroft Way, Edenbridge
Kent TN8 6HE, United Kingdom

phone **44.1732.864001**
fax **44.1732.863356**
e-mail
sales@harvardapparatus.co.uk
website
www.harvardapparatus.co.uk

Authorized Distributors

*The following **Distributors** are available to serve customers outside of the US. They can provide technical assistance, catalog information and quotations (including shipping and importation costs) and after sales service. Some distributors maintain a stock of products for fast delivery. If no distributor is listed for your country, contact any Harvard Apparatus office for information.*

ARGENTINA

ETC International SA
Allende 3274
Ciudad Autonoma de Buenos Aires
Argentina, C1417BMV

phone **54.11.4639.3488**
fax **54.11.4639.6771**
e-mail **etcint@etc.com.ar**

AUSTRALIA

SDR Clinical Technology
213 Eastern Valley Way,
Middle Cove, NSW 2068, Australia

phone **61.02.9958.2688**
fax **61.02.9958.2655**
e-mail **sdr@sdr.com.au**
website **www.sdr.com.au**

BRAZIL

Sellex, Inc.
R. Cardoso de Almedia 788-114/S-1
05013-001 Sâo Paulo – SP Brazil

phone **55.11.3872.2015**
fax **55.11.3872.1024**
e-mail **saopaulo@sellex.com**
website **www.sellex.com**

CHILE

Del Carpio Analisisy Asesorias Ltda
Avda Sucre #2596
Nunoa Santiago, Chile

phone **56.2.269.1348**
fax **56.2.341.5397**
e-mail **enazir@delcarpio.cl**
website **www.delcarpio.cl**

CHINA / HONG KONG

Bioprobes Ltd.
Room 702, 7/F, Knutsford
Communications Building
4-5 Knutsford Terrace TST
KLN Hong Kong

phone **852.2723.9888**
fax **852.2724.2633**
e-mail **info@bioprobes.biz.com.hk**

INDIA

Marsap Services Pvt. Ltd.
29/31 Ujagar Ind. Estate
WTP Marg Rd.
Deonar, Mumbai, India 400 088

phone **91.22.2551.6908**
fax **91.22.2556.3356**
e-mail **marsap@vsnl.com**

ISRAEL

New Biotechnology Ltd.
P.O. Box 8662
Jerusalem, 91086, Israel

phone **972.2.6732001**
fax **972.2.6731611**
e-mail **nbtsales@inter.net.il**

ITALY

Crisel Penco
Clivo di Cinna, 196
00136 Roma, Italy

phone **39.06.35402933**
fax **39.06.35402879**
e-mail **penco@crisel-instruments.it**
website **www.crisel-instruments.it**

JAPAN

Take-In Incorporated
Kyosu Building 3-31-11 Amanuma
Suginami, Tokyo 167-0032, Japan

phone **81.3.3597.1911**
fax **81.3.5833.5596**
e-mail **info@ha-j.com**
website **www.ha-j.com**

PORTUGAL/SPAIN

Izasa S.A.
C/ Aragon 90
0815 Barcelona, Spain

phone **34.902.20.30.80**
fax **34.902.20.30.81**
e-mail **dac2@izasa.es**
website **www.izasa.es**

SOUTH KOREA

Scitech Korea
40-5 Wooi-dong
Kangbuk-ku 142-871, Korea

phone **82.02.999.4419**
fax **82.02.999.4416**
e-mail **scitech@kornet.net**

TAIWAN

Major Instruments Co. Ltd.
6th Floor No. 69-4
Chung-Cheng E. Rd., Sec. 2
Tan-Shui, Taipei, Taiwan, ROC

phone **886.02.2808.1452**
fax **886.02.2808.2354**
e-mail **majortw@ms6.hinet.net**
website **www.major.com.tw**

specialized tools for Electrophysiology and Cell Biology research

Chambers

Imaging and Recording Chambers

Chambers for live cell microscopy, Series 20, 30, 40, and 50. Culture Dish Inserts, Heated Platforms, Stage Adapters and Chamber Accessories

Perfusion

Perfusion

Syringe & Peristaltic Pumps, Valve Control Systems, Fast-Step Perfusion Systems, Gas Controllers, Spill Detection Systems and Accessories

Temperature Control

Temperature Control

Low Noise Temperature Controllers, In-Line Solution Heaters and Coolers, Objective and Syringe Warmers, Thermistors, Cables, and Accessories

Micro-Incubation

Micro-Incubation

Heated Culture Dish Platforms for 35 and 50 mm Dishes, Heated Platform for Chambered Slides, Glass Bottom Cell Culture Dishes, Brain Slice Chamber System

Electrophysiology Equipment

Electrophysiology Equipment

Patch Clamp Equipment, Bilayer Workstation, Oocyte Clamps, Amplifiers, Low Pass Filters, Neurolog™ System, Ussing/Diffusion, Stimulators

Electrophysiology Tools

Electrophysiology Tools

Capillary Glass, Pipette Pullers and Microforges, Microelectrode Holders, Micropositioning, Isolation Equipment

Biosensing

Biosensing

Nitric Oxide Systems, Dissolved O_2, Respirometry, Electrodes, Books

Cell Biology Tools

Cell Biology Tools

Microinjection, Tissue Sampling, Microscopes, Illuminators

Indexes

Indexes

Warner Model Number Index
Ordering Number Index
Product Index

WARNER INSTRUMENTS

A Harvard Apparatus Company

1125 Dixwell Avenue
Hamden, CT 06514 USA

Phone: (800) 599-4203 (toll-free)
(203) 776-0664

Fax: (203) 776-1278

E-mail: support@warneronline.com

HARVARD APPARATUS

84 October Hill Road
Holliston, MA 01746-1388 USA

Phone: (800) 272-2775 (toll-free)
(508) 893-8999

Fax: (508) 429-5732

E-mail: bioscience@harvardapparatus.com

Presorted
Bound Printed Matter
U.S. Postage
PAID
Harvard Apparatus

Harvard Apparatus
84 October Hill Road
Holliston, MA 01746-1388 USA

Address Service Requested